


# INSTRUCTION MANUAL



## Model 109 Temperature Probe

Revision: 3/16

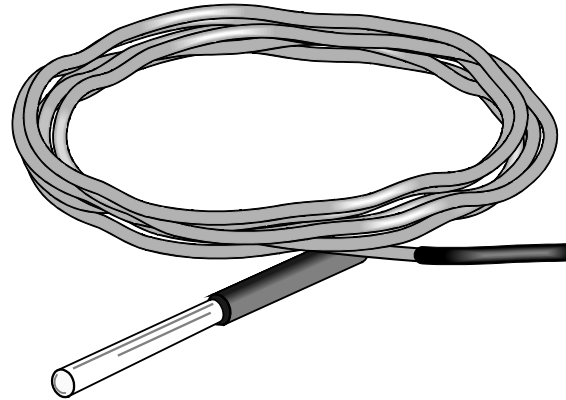

Copyright © 1983-2016  
Campbell Scientific, Inc.



# ***Limited Warranty***

---

“Products manufactured by CSI are warranted by CSI to be free from defects in materials and workmanship under normal use and service for twelve months from the date of shipment unless otherwise specified in the corresponding product manual. (Product manuals are available for review online at [www.campbellsci.com](http://www.campbellsci.com).) Products not manufactured by CSI, but that are resold by CSI, are warranted only to the limits extended by the original manufacturer. Batteries, fine-wire thermocouples, desiccant, and other consumables have no warranty. CSI’s obligation under this warranty is limited to repairing or replacing (at CSI’s option) defective Products, which shall be the sole and exclusive remedy under this warranty. The Customer assumes all costs of removing, reinstalling, and shipping defective Products to CSI. CSI will return such Products by surface carrier prepaid within the continental United States of America. To all other locations, CSI will return such Products best way CIP (port of entry) per Incoterms ® 2010. This warranty shall not apply to any Products which have been subjected to modification, misuse, neglect, improper service, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied. The warranty for installation services performed by CSI such as programming to customer specifications, electrical connections to Products manufactured by CSI, and Product specific training, is part of CSI’s product warranty. **CSI EXPRESSLY DISCLAIMS AND EXCLUDES ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. CSI hereby disclaims, to the fullest extent allowed by applicable law, any and all warranties and conditions with respect to the Products, whether express, implied or statutory, other than those expressly provided herein.”**

# Assistance

---

Products may not be returned without prior authorization. The following contact information is for US and international customers residing in countries served by Campbell Scientific, Inc. directly. Affiliate companies handle repairs for customers within their territories. Please visit [www.campbellsci.com](http://www.campbellsci.com) to determine which Campbell Scientific company serves your country.

To obtain a Returned Materials Authorization (RMA), contact CAMPBELL SCIENTIFIC, INC., phone (435) 227-9000. After an application engineer determines the nature of the problem, an RMA number will be issued. Please write this number clearly on the outside of the shipping container. Campbell Scientific's shipping address is:

**CAMPBELL SCIENTIFIC, INC.**

RMA# \_\_\_\_\_  
815 West 1800 North  
Logan, Utah 84321-1784

For all returns, the customer must fill out a "Statement of Product Cleanliness and Decontamination" form and comply with the requirements specified in it. The form is available from our website at [www.campbellsci.com/repair](http://www.campbellsci.com/repair). A completed form must be either emailed to [repair@campbellsci.com](mailto:repair@campbellsci.com) or faxed to (435) 227-9106. Campbell Scientific is unable to process any returns until we receive this form. If the form is not received within three days of product receipt or is incomplete, the product will be returned to the customer at the customer's expense. Campbell Scientific reserves the right to refuse service on products that were exposed to contaminants that may cause health or safety concerns for our employees.

# Safety

---

**DANGER — MANY HAZARDS ARE ASSOCIATED WITH INSTALLING, USING, MAINTAINING, AND WORKING ON OR AROUND TRIPODS, TOWERS, AND ANY ATTACHMENTS TO TRIPODS AND TOWERS SUCH AS SENSORS, CROSSARMS, ENCLOSURES, ANTENNAS, ETC. FAILURE TO PROPERLY AND COMPLETELY ASSEMBLE, INSTALL, OPERATE, USE, AND MAINTAIN TRIPODS, TOWERS, AND ATTACHMENTS, AND FAILURE TO HEED WARNINGS, INCREASES THE RISK OF DEATH, ACCIDENT, SERIOUS INJURY, PROPERTY DAMAGE, AND PRODUCT FAILURE. TAKE ALL REASONABLE PRECAUTIONS TO AVOID THESE HAZARDS. CHECK WITH YOUR ORGANIZATION'S SAFETY COORDINATOR (OR POLICY) FOR PROCEDURES AND REQUIRED PROTECTIVE EQUIPMENT PRIOR TO PERFORMING ANY WORK.**

Use tripods, towers, and attachments to tripods and towers only for purposes for which they are designed. Do not exceed design limits. Be familiar and comply with all instructions provided in product manuals. Manuals are available at [www.campbellsci.com](http://www.campbellsci.com) or by telephoning (435) 227-9000 (USA). You are responsible for conformance with governing codes and regulations, including safety regulations, and the integrity and location of structures or land to which towers, tripods, and any attachments are attached. Installation sites should be evaluated and approved by a qualified engineer. If questions or concerns arise regarding installation, use, or maintenance of tripods, towers, attachments, or electrical connections, consult with a licensed and qualified engineer or electrician.

## General

- Prior to performing site or installation work, obtain required approvals and permits. Comply with all governing structure-height regulations, such as those of the FAA in the USA.
- Use only qualified personnel for installation, use, and maintenance of tripods and towers, and any attachments to tripods and towers. The use of licensed and qualified contractors is highly recommended.
- Read all applicable instructions carefully and understand procedures thoroughly before beginning work.
- Wear a **hardhat** and **eye protection**, and take **other appropriate safety precautions** while working on or around tripods and towers.
- **Do not climb** tripods or towers at any time, and prohibit climbing by other persons. Take reasonable precautions to secure tripod and tower sites from trespassers.
- Use only manufacturer recommended parts, materials, and tools.

## Utility and Electrical

- **You can be killed** or sustain serious bodily injury if the tripod, tower, or attachments you are installing, constructing, using, or maintaining, or a tool, stake, or anchor, come in **contact with overhead or underground utility lines**.
- Maintain a distance of at least one-and-one-half times structure height, 20 feet, or the distance required by applicable law, **whichever is greater**, between overhead utility lines and the structure (tripod, tower, attachments, or tools).
- Prior to performing site or installation work, inform all utility companies and have all underground utilities marked.
- Comply with all electrical codes. Electrical equipment and related grounding devices should be installed by a licensed and qualified electrician.

## Elevated Work and Weather

- Exercise extreme caution when performing elevated work.
- Use appropriate equipment and safety practices.
- During installation and maintenance, keep tower and tripod sites clear of un-trained or non-essential personnel. Take precautions to prevent elevated tools and objects from dropping.
- Do not perform any work in inclement weather, including wind, rain, snow, lightning, etc.

## Maintenance

- Periodically (at least yearly) check for wear and damage, including corrosion, stress cracks, frayed cables, loose cable clamps, cable tightness, etc. and take necessary corrective actions.
- Periodically (at least yearly) check electrical ground connections.

WHILE EVERY ATTEMPT IS MADE TO EMBODY THE HIGHEST DEGREE OF SAFETY IN ALL CAMPBELL SCIENTIFIC PRODUCTS, THE CUSTOMER ASSUMES ALL RISK FROM ANY INJURY RESULTING FROM IMPROPER INSTALLATION, USE, OR MAINTENANCE OF TRIPODS, TOWERS, OR ATTACHMENTS TO TRIPODS AND TOWERS SUCH AS SENSORS, CROSSARMS, ENCLOSURES, ANTENNAS, ETC.



# Table of Contents

---

PDF viewers: These page numbers refer to the printed version of this document. Use the PDF reader bookmarks tab for links to specific sections.

<b>1. Introduction .....</b>	<b>1</b>
<b>2. Precautions .....</b>	<b>1</b>
<b>3. Initial Inspection.....</b>	<b>1</b>
<b>4. QuickStart.....</b>	<b>1</b>
<b>5. Overview.....</b>	<b>4</b>
<b>6. Specifications.....</b>	<b>4</b>
<b>7. Installation.....</b>	<b>6</b>
7.1 Wiring to Datalogger .....	6
7.2 Datalogger Programming.....	7
7.2.1 Therm109() Instruction.....	7
7.3 Air Temperature Installation.....	8
7.4 Water Temperature Installation.....	10
7.5 Soil Temperature Installation.....	10
<b>8. Operation.....</b>	<b>10</b>
8.1 Sensor Schematic .....	10
8.2 Measurement and Output Linearization.....	10
8.3 Electrically Noisy Environments .....	11
8.4 Long Cable Lengths.....	11
<b>9. Troubleshooting and Maintenance.....</b>	<b>12</b>
9.1 Troubleshooting .....	12
9.2 Maintenance.....	12
9.3 Calibration.....	12
<b>10. Attributions and References .....</b>	<b>13</b>
<b><i>Appendices</i></b>	
<b>A. Importing <i>Short Cut</i> Code Into <i>CRBasic Editor</i> ...</b>	<b>A-1</b>
<b>B. Example Programs.....</b>	<b>B-1</b>
<b>C. Thermistor Resistance and Temperature.....</b>	<b>C-1</b>

**Figures**

6-1. Worst case probe and measurement errors ..... 5  
6-2. Steinhart-Hart linearization error ..... 6  
7-1. Installing a 109 and 41303-5A Radiation Shield on a CM200  
Series Crossarm ..... 9  
7-2. 109 and 41303-5A Radiation Shield on a tripod mast (left).  
109 and RAD06 Radiation Shield on a CM200-series  
Crossarm (right)..... 9  
8-1. 109 Thermistor Probe Schematic ..... 10

**Tables**

7-1. Wire Color, Function, and Datalogger Connection ..... 6  
C-1. 109 Thermistor Resistance and Temperature ..... C-1

**CRBasic Examples**

B-1. Program Example for CR200(X) Series Dataloggers..... B-1  
B-2. Program Example for CR800 Series, CR1000, CR3000, and  
CR5000 Dataloggers ..... B-1  
B-3. Program Example for CR6 Dataloggers..... B-2



# Model 109 Temperature Probe

---

## 1. Introduction

The 109 Temperature Probe uses a thermistor to measure temperature in air, soil, and water. It is compatible with all CRBasic dataloggers except the CR9000(X). See Section 6, *Specifications (p. 4)*, for a list of compatible CRBasic dataloggers.

For Edlog datalogger support, check the availability of an older manual at [www.campbellsci.com/old-manuals](http://www.campbellsci.com/old-manuals), or contact a Campbell Scientific application engineer for assistance.

## 2. Precautions

- READ AND UNDERSTAND the *Safety* section at the front of this manual.
- Santoprene® rubber, which composes the black outer jacket of the 109 cable, will support combustion in air. It is used because of its resistance to temperature extremes, moisture, and UV degradation. It is rated as slow burning when tested according to U.L. 94 H.B. and passes FMVSS302. However, local fire codes may preclude its use inside buildings.

## 3. Initial Inspection


- Check the packaging and contents of the shipment. If damage occurred during transport, immediately file a claim with the carrier. Contact Campbell Scientific to facilitate repair or replacement.
- Check model information against the shipping documents to ensure the expected products and the correct lengths of cable are received. Model numbers are found on each product. On cables and cabled items, the model number is usually found at the connection end of the cable. Report any shortages immediately to Campbell Scientific.

## 4. QuickStart


*Short Cut* is an easy way to program your datalogger to measure the 109 probe and assign datalogger wiring terminals. *Short Cut* is available as a download on [www.campbellsci.com](http://www.campbellsci.com) and the *ResourceDVD*. It is included in installations of *LoggerNet*, *PC200W*, *PC400*, or *RTDAQ*.


Use the following procedure to get started.


1. Open *Short Cut*. Click **New Program**.

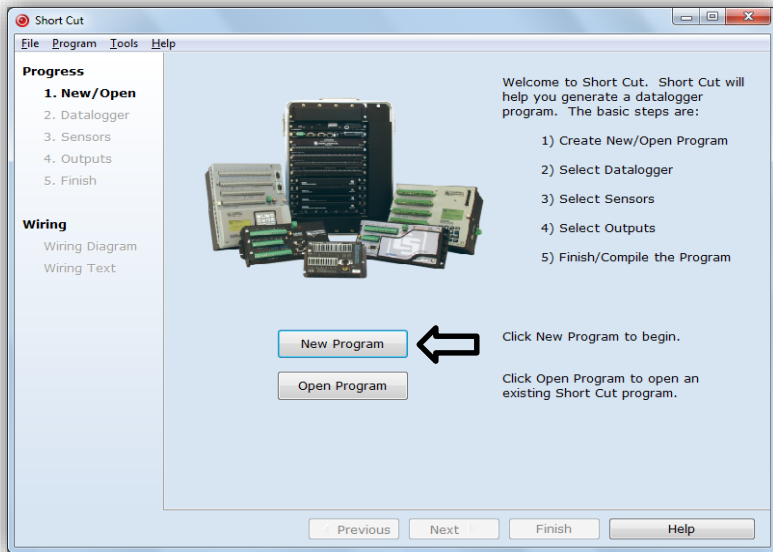


2. Select **Datalogger Model** and **Scan Interval** (default of 5 or 10 seconds is OK for most applications). Click **Next**.

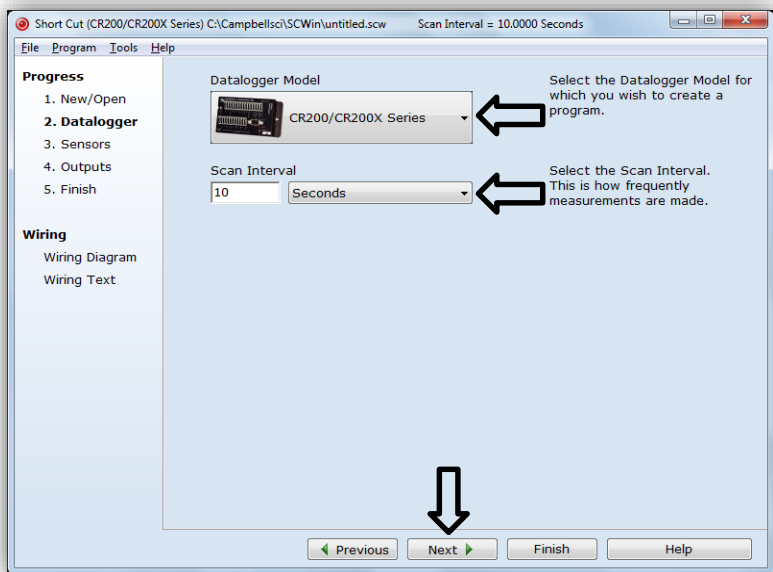

- Under the **Available Sensors and Devices** list, select the **Sensors** folder, then select the **Temperature** sub-folder. Select **109 Temperature Probe**. Click  to move the selection to the **Selected** device window. Data defaults to degree Celsius. This can be changed by clicking the **Deg C** box and selecting **Deg F**, for degrees Fahrenheit, or **K**, for Kelvin.

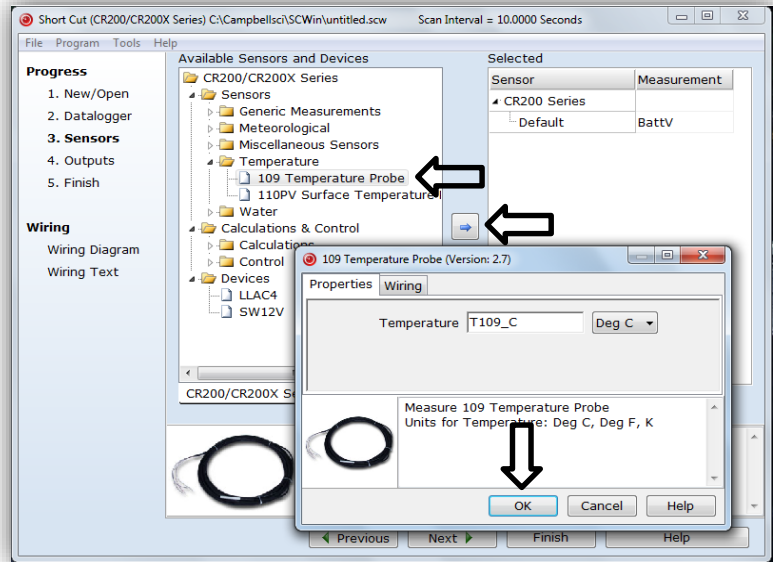

- After selecting the sensor, click **Wiring Diagram** to see how the sensor is to be wired to the datalogger. The wiring diagram can be printed now or after more sensors are added.

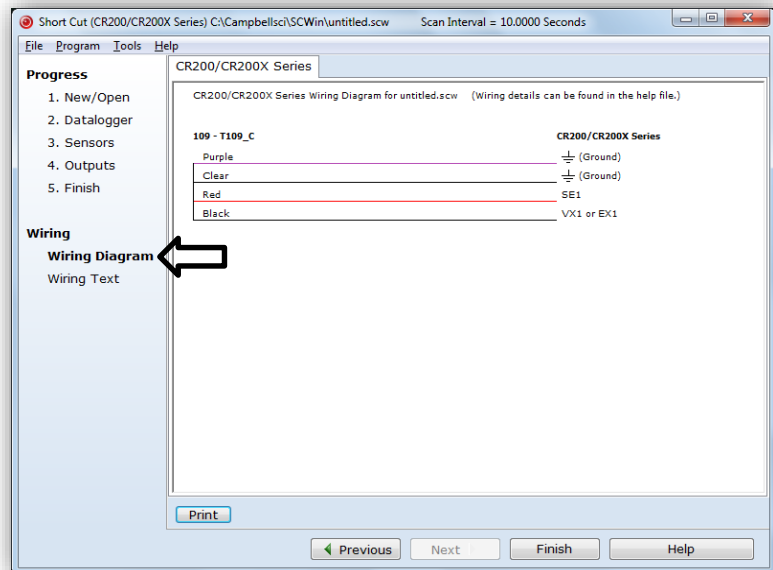

5. Select any other sensors you have, and then finish the remaining *Short Cut* steps to complete the program. The remaining steps are outlined in *Short Cut Help*, which is accessed by clicking on **Help | Contents | Programming Steps**.
6. If *LoggerNet*, *PC400*, *RTDAQ*, or *PC200W* is running on your PC, and the PC to datalogger connection is active, you can click **Finish** in *Short Cut* and you will be prompted to send the program just created to the datalogger.
7. If the sensor is connected to the datalogger, as shown in the wiring diagram in step 4, check the output of the sensor in the datalogger support software data display to make sure it is making reasonable measurements.

## 5. Overview

The 109 is a rugged probe that accurately measures air, soil, or water temperature in a variety of applications. The sensor consists of a thermistor encapsulated in an epoxy-filled aluminum housing. This design allows the probe to be buried or submerged in water to 15 m (50 ft) or 21 psi. When measuring air temperature, a 41303-5A radiation shield is normally used to mount the 109 and limit solar radiation loading. See *Specifications* for a complete list of compatible dataloggers.

## 6. Specifications

### Features:

- Measures air, soil, or water temperature
- Compatible with AM16/32-series multiplexers
- Easy to install or remove
- Durable
- Compatible with the following CRBasic dataloggers: CR6, CR200(X), and CR800 series, CR1000, CR3000, and CR5000

<b>Sensor Element:</b>	Measurement Specialties™ 10K3A1iA thermistor
<b>Survival Range:</b>	-50 to 100 °C
<b>Measurement Range:</b>	-50 to 70 °C
<b>Time Constant in Air:</b>	30 to 60 s in a wind speed of 5 m/s
<b>Maximum Cable Length:</b>	1000 ft
<b>Accuracy<sup>1</sup></b>	
<b>Worst case:</b>	±0.60 °C (-50 to 70 °C) ±0.25 °C (-10 to 70 °C)
<b>Interchangeability Error:</b>	±0.10 °C (0 to 70 °C) ±0.13 °C at -10 °C ±0.15 °C at -20 °C ±0.18 °C at -30 °C ±0.20 °C at -40 °C ±0.50 °C at -50 °C

**Steinhart-Hart  
Linearization Error:**  $\leq 0.03 \text{ }^\circ\text{C}$  (-50 to 70  $^\circ\text{C}$ )

**Probe Weight and Dimensions**

**Weight with 10 ft cable:** 136 g (5 oz)  
**Length:** 10.4 cm (4.1 in)  
**Diameter:** 0.762 cm (0.3 in)

<sup>1</sup>See FIGURE 6-1, *Worst-case probe and measurement errors*, and FIGURE 6-2, *Steinhart-Hart linearization error*. Overall probe accuracy is a combination of thermistor interchangeability, bridge-resistor accuracy, and error of the Steinhart-Hart equation. Interchangeability is the principle component error and is predominantly offset. Offset can be determined with a single-point calibration. Offset can be entered in the **Therm109()** instruction **Offset** parameter. The bridge resistor has a 0.1% tolerance with a 10 ppm temperature coefficient. At temperature extremes, the possible error in the CR200(X) series datalogger measurement may be greater than the error that exists in the probe.

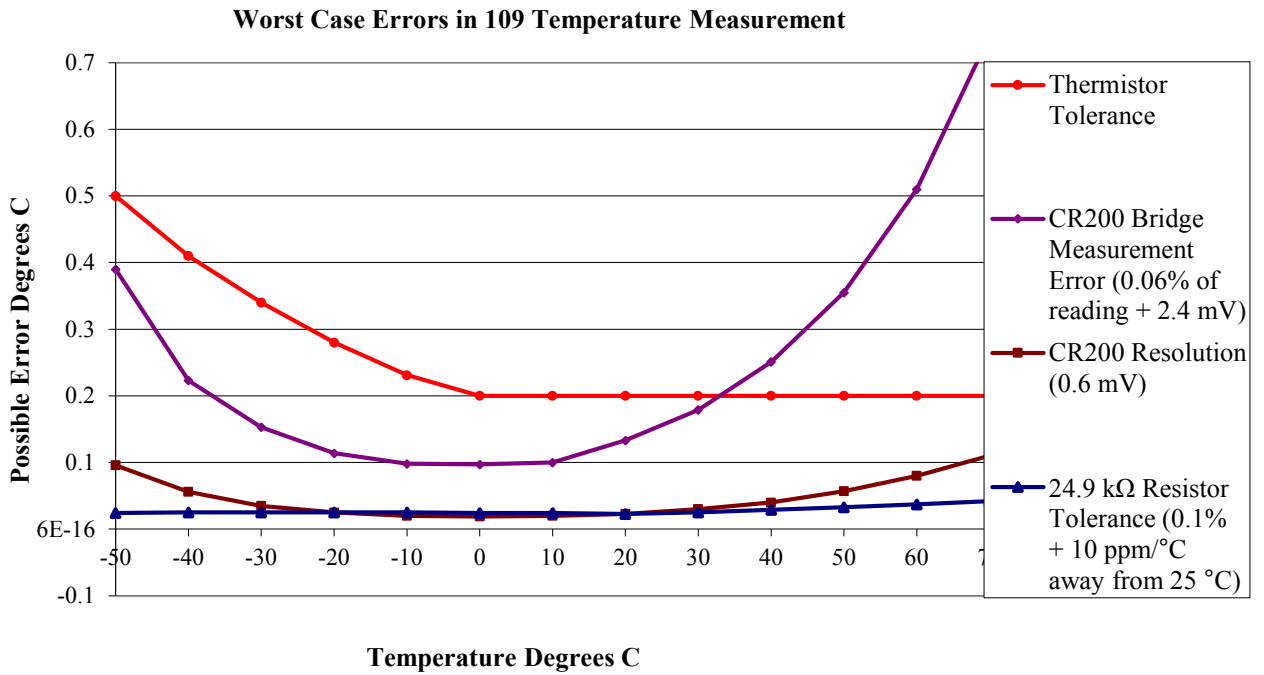


FIGURE 6-1. Worst case probe and measurement errors

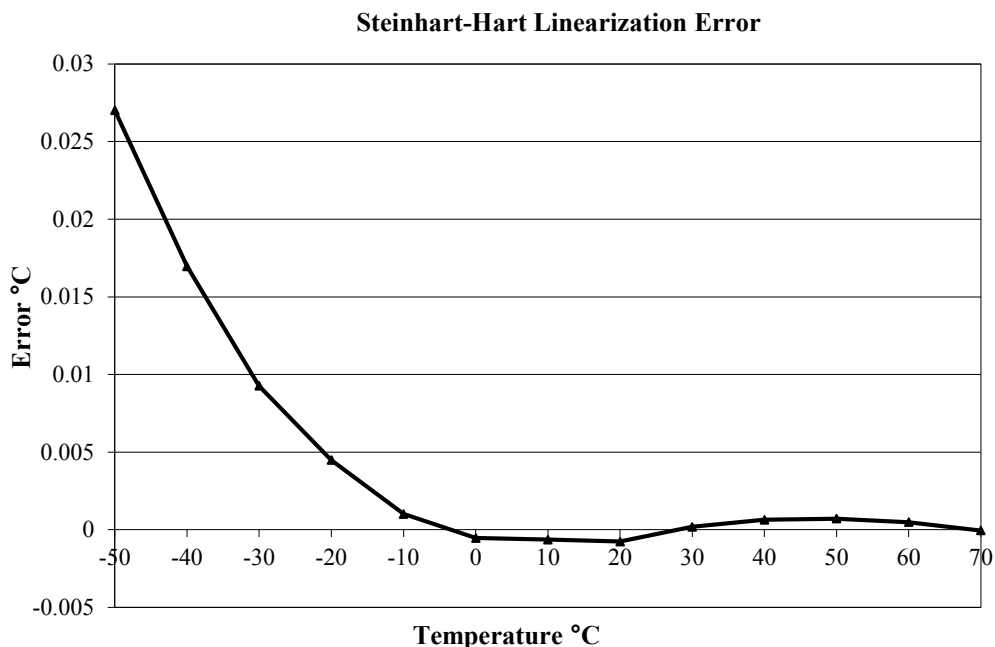




FIGURE 6-2. Steinhart-Hart linearization error

## 7. Installation

If you are programming your datalogger with *Short Cut*, skip Section 7.1, *Wiring to Datalogger* (p. 6), and Section 7.2, *Datalogger Programming* (p. 7). *Short Cut* does this work for you. See Section 4, *QuickStart* (p. 1), for a *Short Cut* tutorial.

### 7.1 Wiring to Datalogger

Wire Color	Wire Function	Datalogger Connection Terminal
Black	Voltage-excitation input	U configured for voltage excitation <sup>1</sup> , <b>EX</b> , <b>VX</b> (voltage excitation)
Red	Analog-voltage output	U configured for single-ended analog input <sup>1</sup> , <b>SE</b> (single-ended, analog-voltage input)
Purple	Bridge-resistor lead	<b>AG</b> or  (analog ground)
Clear	EMF shield	<b>AG</b> or  (analog ground)
<sup>1</sup> U channels are automatically configured by the measurement instruction.		

## 7.2 Datalogger Programming

*Short Cut* is the best source for up-to-date datalogger programming code. Programming code is needed when:

- Creating a program for a new datalogger installation
- Adding sensors to an existing datalogger program

If your data acquisition requirements are simple, you can probably create and maintain a datalogger program exclusively with *Short Cut*. If your data acquisition needs are more complex, the files that *Short Cut* creates are a great source for programming code to start a new program or add to an existing custom program.

### NOTE

*Short Cut* cannot edit programs after they are imported and edited in *CRBasic Editor*.

A *Short Cut* tutorial is available in Section 4, *QuickStart* (p. 1). If you wish to import *Short Cut* code into *CRBasic Editor* to create or add to a customized program, follow the procedure in Appendix A, *Importing Short Cut Code Into CRBasic Editor* (p. A-1). Programming basics are provided in the following section. A complete program example can be found in Appendix B, *Example Programs* (p. B-1).

If the 109 probe is to be used with long cable lengths or in electrically noisy environments, consider employing the measurement programming techniques outlined in Section 8.3, *Electrically Noisy Environments* (p. 11), and Section 8.4, *Long Cable Lengths* (p. 11).

Details of 109 probe measurement and linearization of the thermistor output are provided in Section 8.2, *Measurement and Output Linearization* (p. 10).

### 7.2.1 Therm109() Instruction

The **Therm109()** measurement instruction programs most CRBasic dataloggers (CR6-, CR200(X)-, and CR800-series, CR1000, CR3000, and CR5000) to measure the 109 probe. It applies a precise excitation voltage, makes a half-bridge resistance measurement, and converts the result to temperature using the Steinhart-Hart equation. See Section 8.2, *Measurement and Output Linearization* (p. 10), for more information. **Therm109()** instruction and parameters are as follows:

**Therm109**(Dest, Reps, SEChan, VxChan, SettlingTime, Integ/Fnotch, Mult, Offset)

The instruction for CR200(X) series dataloggers excludes the *SettlingTime* and *Integ* parameters.

Variations:

- Temperature reported as °C — set **Mult** to **1** and **Offset** to **0**
- Temperature reported as °F — set **Mult** to **1.8** and **Offset** to **32**
- AC mains noise filtering — set **Integ/Fnotch** to **\_60Hz** or **\_50Hz** (see Section 8.3, *Electrically Noisy Environments* (p. 11))
- Compensate for long cable lengths — Set **SettlingTime** to **20000** (see Section 8.4, *Long Cable Lengths* (p. 11))

## 7.3 Air Temperature Installation

For air temperature measurements, locate probes over an open level area at least 9 m (EPA) in diameter. The surface should be covered by short grass or the natural earth surface where grass does not grow. Probes should be located at a distance of at least four times the height of any nearby obstruction, and at least 30 m (EPA) from large paved areas. Sensors should be protected from thermal radiation, and adequately ventilated.

Standard air temperature measurement heights:

- 1.25 to 2.0 m (WMO)
- 2.0 m (EPA)
- 2.0 m and 10.0 m for temperature difference (EPA)

When exposed to sunlight, the 109 should be housed in a six-plate solar radiation shield. Six-plate shields offered by Campbell Scientific are models 41303-5A, 41303-5B, or RAD06.

The white color of these shields reflects solar radiation, and the louvered construction allows air to pass freely through, thereby keeping the probe at or near ambient temperature. The RAD06 uses a double-louvered design that offers improved sensor protection from insect intrusion and driving rain and snow. In addition, the RAD06 shield has lower self-heating in bright sunlight combined with higher temperatures ( $> 24\text{ }^{\circ}\text{C}$  ( $75\text{ }^{\circ}\text{F}$ )) and low wind speeds ( $< 2\text{ m/s}$  ( $4.5\text{ mph}$ )), giving a better measurement.

The 41303-5A and RAD06 attach to a crossarm, mast, or user-supplied pipe with a 2.5 to 5.3 cm (1.0 to 2.1 in) outer diameter. The 41303-5B attaches to a CM500-series pole or a user-supplied pole with a 5.1 cm (2.4 in) outer diameter.

Tools required for installing a radiation shield to a tripod or tower include:

- 1/2 inch open end wrench
- small screw driver provided with datalogger
- small Phillips screwdriver
- UV resistant cable ties
- small pair of diagonal-cutting pliers
- adjustable wrench with a minimum 1-1/2 inch jaw size





*FIGURE 7-1. Installing a 109 and 41303-5A Radiation Shield on a CM200 Series Crossarm*



*FIGURE 7-2. 109 and 41303-5A Radiation Shield on a tripod mast (left). 109 and RAD06 Radiation Shield on a CM200-series Crossarm (right).*

The 109 is held in the 41303-5A radiation shield by a mounting clamp at the bottom (FIGURE 7-1 and FIGURE 7-2 left). Loosen the mounting clamp screws, and insert the probe through the clamp. Tighten the screws to secure the sensor, and route the sensor cable to the instrument enclosure.

The 109 is held in the RAD06 radiation shield by inserting the sensor through the sensor gland at the bottom of the shield (FIGURE 7-2 right). Loosen the nut on the gland, and insert the probe into the shield. Tighten the nut on the sensor gland using an adjustable wrench until the sensor is securely held in place. Route the sensor cable to the instrument enclosure.

Secure the cable to the tripod or tower using cable ties.

## 7.4 Water Temperature Installation

109 probes can be submerged to 15 m (50 ft) or 21 psi. The 109 is not weighted, so a weighting system should be added, or the probe secured to a submerged object such as a piling.

## 7.5 Soil Temperature Installation

The 109 tends to measure the average temperature over its length, so burying the probe such that the measurement tip is horizontal to the soil surface at the desired depth is usually preferred. The maximum burial depth for soil that could become saturated with water is dictated by the maximum water pressure allowed for the sensor, which is 21 psi.

One or two coils of cable should also be buried in a shallow installation. Burial of some cable mitigates the effect of solar heating of the above ground cable on the temperature measurement.

Placement of the cable inside a rugged conduit may be necessary for long cable runs, especially in locations subject to digging, mowing, traffic, use of power tools, or lightning strikes.

# 8. Operation

## 8.1 Sensor Schematic

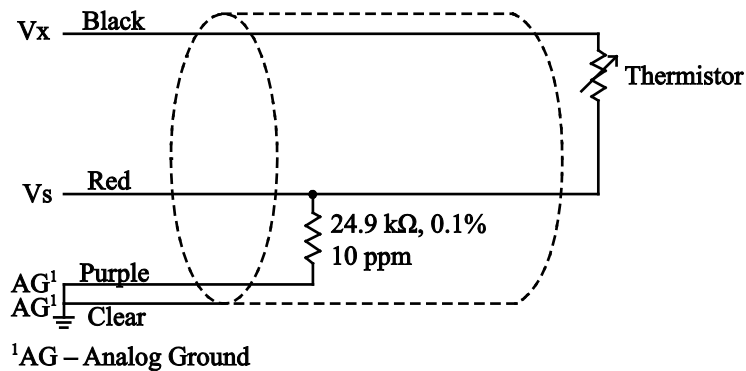


FIGURE 8-1. 109 Thermistor Probe Schematic

## 8.2 Measurement and Output Linearization

CRBasic instruction **Therm109()** measures the 109 probe thermistor and automatically converts the result to temperature. With reference to the previous FIGURE 8-1, *109 Thermistor Probe Schematic*, **Therm109()** applies 2500 mV excitation at the Vx line and measures the voltage drop across the 24.9 kΩ resistor at the Vs line.

The ratio of measured voltage ( $V_s$ ) to excitation voltage ( $V_x$ ) is related to thermistor resistance ( $R_s$ ) and the 24.9 k $\Omega$  bridge resistor as described in the following equations:

$$V_s/V_x = 24900 \Omega / (R_s + 24900 \Omega)$$

Solving for  $R_s$ :

$$R_s + 24900 \Omega = 24900 \Omega \cdot (V_x/V_s)$$

$$R_s = 24900 \Omega \cdot ((V_x/V_s) - 1)$$

The relationship of  $R_s$  to temperature is tabulated in Appendix C, *Thermistor Resistance and Temperature (p. C-1)*, but is calculated by **Therm109()** using the Steinhart-Hart equation, described as follows:

$$T_c = (1 / (A + B \cdot \ln(R_s) + C \cdot (\ln(R_s))^3)) - 273.15$$

where:

$T_c$  = temperature in degrees Celsius ( $^{\circ}\text{C}$ )

$$A^1 = 1.129241\text{E-}3$$

$$B^1 = 2.341077\text{E-}4$$

$$C^1 = 8.775468\text{E-}8$$

<sup>1</sup>Coefficients provided by Measurement Specialties™.

### 8.3 Electrically Noisy Environments

EMF noise emanating from the ac mains power grid can be a significant source of measurement error. 60 Hz noise is common in the United States. 50 Hz noise is common in Europe and other regions. Depending on the datalogger model, this noise can usually be filtered out.

The following code snips filter 60 Hz noise by placing the **\_60Hz** argument in the **Integ/Fnotch** parameter (in bold type).

For CR6 datalogger:

```
Therm109(T109_C, 1, U1, U10, 20000, _60Hz, 1.0, 0.0)
```

For CR800, CR1000, CR3000, and CR5000 dataloggers:

```
Therm109(T109_C, 1, 1, 1, 20000, _60Hz, 1.0, 0.0)
```

An integration parameter is not available for CR200(X) series dataloggers.

### 8.4 Long Cable Lengths

Long cable lengths may require longer than normal analog measurement settling times. Settling times are increased by adding a measurement delay to a datalogger program.

The 60 Hz and 50 Hz integration options include a 3 ms settling time; longer settling times can be entered into the **Settling Time** parameter. The following code snips increase settling time by 20000  $\mu\text{s}$  by placing **20000** as the argument in the **SettlingTime** parameter:

For CR6 datalogger:

```
Therm109(T109_C,1,U1,U10,20000,_60Hz,1.0,0.0)
```

For CR800, CR1000, CR3000, and CR5000 dataloggers:

```
Therm109(T109_C,1,1,1,20000,_60Hz,1.0,0.0)
```

A setting time parameter is not available for CR200(X) series dataloggers.

## 9. Troubleshooting and Maintenance

### NOTE

---

All factory repairs and recalibrations require a returned material authorization (RMA) and completion of the “Declaration of Hazardous Material and Decontamination” form. Refer to the [Assistance](#) page at the beginning of this manual for more information.

---

### 9.1 Troubleshooting

Symptom: Temperature is reported as **NAN**, **-INF**, or incorrect temperature.

Verify wire leads are connected to the terminals specified in the **Therm109()** instruction: red to single-ended analog input (**SE** or **U**), black to switched excitation (**VX/EX** or **U**), and purple to ground ( $\perp$ ).

Symptom: Incorrect temperature is reported.

Verify the **Mult** and **Offset** arguments in **Therm109()** are correct for the desired units (Section 7.2, *Datalogger Programming* (p. 7)). Check the cable for signs of damage and possible moisture intrusion.

Symptom: Unstable temperature is reported.

Probably a result of electromagnetic interference. Try using the **\_50Hz** or **\_60Hz Integ** or **Fnotch** options, and/or increasing the settling time as described in Section 8.3, *Electrically Noisy Environments* (p. 11), and Section 8.4, *Long Cable Lengths* (p. 11). Ensure the clear wire is connected to datalogger ground, and the datalogger is properly grounded.

### 9.2 Maintenance

The 109 probe requires minimal maintenance. For air temperature measurements, check the radiation shield monthly to make sure it is clean and free from debris. Periodically check cabling for signs of damage and possible moisture intrusion.

### 9.3 Calibration

Calibration of the 109 probe is not necessary unless the application requires removal of the thermistor interchangeability offset described in Section 6, *Specifications* (p. 4).

## 10. Attributions and References

Santoprene® is a registered trademark of Exxon Mobile Corporation.

Measurement Specialties™ is a trademarked global designer and manufacturer of sensors and sensor-based systems.

EPA installation standard: *Quality Assurance Handbook for Air Pollution Measurement Systems – Volume IV: Meteorological Measurements Version 2.0*

WMO standard: *WMO No. 8, Seventh edition, 6 Aug 2008 Guide to Meteorological Instruments and Methods of Observation*



# Appendix A. Importing Short Cut Code Into CRBasic Editor

---

This tutorial shows:

- How to import a *Short Cut* program into a program editor for additional refinement
- How to import a wiring diagram from *Short Cut* into the comments of a custom program

*Short Cut* creates files, which can be imported into *CRBasic Editor*. Assuming defaults were used when *Short Cut* was installed, these files reside in the C:\campbellsci\SCWin folder:

- .DEF (wiring and memory usage information)
- .CR6 (CR6 datalogger code)
- .CR1 (CR1000 datalogger code)
- .CR2 (CR200X datalogger code)
- .CR8 (CR800 datalogger code)
- .CR3 (CR3000 datalogger code)
- .CR5 (CR5000 datalogger code)

Use the following procedure to import *Short Cut* code and wiring diagram into *CRBasic Editor*.

1. Create the *Short Cut* program following the procedure in Section 4, *QuickStart* (p. 1). Finish the program and exit *Short Cut*. Make note of the file name used when saving the *Short Cut* program.
2. Open *CRBasic Editor*.
3. Click **File | Open**. Assuming the default paths were used when *Short Cut* was installed, navigate to C:\CampbellSci\SCWin folder. The file of interest has the .CR6, .CR1, .CR2, .CR8, .CR3, or .CR5 extension. Select the file and click **Open**.
4. Immediately save the file in a folder different from C:\Campbellsci\SCWin, or save the file with a different file name.

---

## NOTE

Once the file is edited with *CRBasic Editor*, *Short Cut* can no longer be used to edit the datalogger program. Change the name of the program file or move it, or *Short Cut* may overwrite it next time it is used.

---

5. The program can now be edited, saved, and sent to the datalogger.
6. Import wiring information to the program by opening the associated .DEF file. Copy and paste the section beginning with heading “-Wiring for CRXXX-” into the CRBasic program, usually at the head of the file. After pasting, edit the information such that an apostrophe (') begins each line.

This character instructs the datalogger compiler to ignore the line when compiling.



# Appendix B. Example Programs

The following example can be used directly with CR200(X) series dataloggers.

## CRBasic Example B-1. Program Example for CR200(X) Series Dataloggers

```
'Program measures one 109 temperature probe once a second and
'stores the average temperature every 60 minutes.

'Wiring Diagram
'=====
' 109
' Probe
' Lead                               CR200(X)
' Color      Function                Terminal
' -----
' Black      Voltage-excitation input  VX1/EX1
' Red        Analog-voltage output     SE1
' Purple     Bridge-resistor ground    Ground Symbol
' Clear      Shield                    Ground Symbol

'Declare the variable for the temperature measurement
Public T109_C

'Define a data table for 60 minute averages
DataTable(Table1,True,-1)
  DataInterval(0,60,min)
  Average(1,T109_C,False)
EndTable

BeginProg
  Scan(1,sec)
    'Measure the temperature
    Therm109(T109_C,1,1,Ex1,1.0,0)
    'Call Data Table
    CallTable Table1
  NextScan
EndProg
```

This following example can be used directly with CR800 series, CR1000, CR3000, and CR5000 dataloggers.

## CRBasic Example B-2. Program Example for CR800 Series, CR1000, CR3000, and CR5000 Dataloggers

```
'Program measures one 109 temperature probe once a second and
'stores the average temperature every 60 minutes.

'Wiring Diagram
'=====
' 109
' Probe
' Lead                               CR1000
' Color      Function                Terminal
' -----
' Black      Voltage-excitation input  VX1 or EX1
' Red        Analog-voltage output     SE1
' Purple     Bridge-resistor ground    Ground Symbol
' Clear      Shield                    Ground Symbol

'Declare the variables for the temperature measurement
Public T109_C
```

```

'Define a data table for 60 minute averages:
DataTable(Table1,True,-1)
  DataInterval(0,60,Min,0)
  Average(1,T109_C,IEEE4,0)
EndTable

BeginProg
  Scan(1,Sec,1,0)
    'Measure the temperature
    Therm109(T109_C,1,1,Vx1,0,_60Hz,1.0,0.0)
    'Call Data Table
    CallTable(Table1)
  NextScan
EndProg

```

The following example can be used directly with CR6 series dataloggers.

### CRBasic Example B-3. Program Example for CR6 Dataloggers

```

'Program measures one 109 temperature probe once a second and
'stores the average temperature every 60 minutes.

'Wiring Diagram
'=====
' 109
' Probe
' Lead
' Color      Function
' -----
' Black      Voltage-excitation input
' Red        Analog-voltage output
' Purple     Bridge-resistor ground
' Clear      Shield
' CR6
' Terminal
' -----
' U10
' U1
' Ground Symbol
' Ground Symbol

'Declare the variables for the temperature measurement
Public T109_C

'Define a data table for 60 minute averages:
DataTable(Table1,True,-1)
  DataInterval(0,60,Min,0)
  Average(1,T109_C,IEEE4,0)
EndTable

BeginProg
  Scan(1,Sec,1,0)
    'Measure the temperature
    Therm109(T109_C,1,U1,U10,0,_60Hz,1.0,0.0)
    'Call Data Table
    CallTable(Table1)
  NextScan
EndProg

```

# Appendix C. Thermistor Resistance and Temperature

---

TABLE C-1. 109 Thermistor Resistance and Temperature<sup>1</sup>

Actual Temperature (°C)	10K3A1iA Thermistor Resistance (Ω)	CRBasic Therm109() Output (°C)
-40	336098	-40.00
-39	314553	-39.00
-38	294524	-38.00
-37	275897	-37.00
-36	258563	-36.00
-35	242427	-35.00
-34	227398	-34.00
-33	213394	-33.00
-32	200339	-32.00
-31	188163	-31.00
-30	176803	-30.00
-29	166198	-29.00
-28	156294	-28.00
-27	147042	-27.00
-26	138393	-26.00
-25	130306	-25.00
-24	122741	-24.00
-23	115661	-23.00
-22	109032	-22.00
-21	102824	-21.00
-20	97006	-20.00
-19	91553	-19.00
-18	86439	-18.00
-17	81641	-17.00
-16	77138	-16.00
-15	72911	-15.00
-14	68940	-14.00
-13	65209	-13.00
-12	61703	-12.00
-11	58405	-11.00
-10	55304	-10.00
-9	52385	-9.00
-8	49638	-8.00
-7	47050	-7.00
-6	44613	-6.00
-5	42317	-5.00
-4	40151	-4.00
-3	38110	-3.00
-2	36184	-2.00
-1	34366	-1.00
0	32651	0.00
1	31031	1.00
2	29500	2.00
3	28054	3.00

Appendix C. Thermistor Resistance and Temperature

4	26687	4.00
5	25395	5.00
6	24172	6.00
7	23016	7.00
8	21921	8.00
9	20885	9.00
10	19903	10.00
11	18973	11.00
12	18092	12.00
13	17257	13.00
14	16465	14.00
15	15714	15.00
16	15001	16.00
17	14324	17.00
18	13682	18.00
19	13073	19.00
20	12493	20.00
21	11943	21.00
22	11420	22.00
23	10923	23.00
24	10450	24.00
25	10000	25.00
26	9572	26.00
27	9165	27.00
28	8777	28.00
29	8408	29.00
30	8056	30.00
31	7721	31.00
32	7402	32.00
33	7097	33.00
34	6807	34.00
35	6530	35.00
36	6266	36.00
37	6014	37.00
38	5774	38.00
39	5544	39.00
40	5325	40.00
41	5116	41.00
42	4916	42.00
43	4724	43.00
44	4542	44.00
45	4367	45.00
46	4200	46.00
47	4040	47.00
48	3887	48.00
49	3741	49.00
50	3601	50.00
51	3467	51.00
52	3339	52.00
53	3216	53.00
54	3098	54.00
55	2985	55.00
56	2877	56.00
57	2773	57.00
58	2674	58.00
59	2579	59.00

60	2487	60.00
61	2399	61.00
62	2315	62.00
63	2234	63.01
64	2157	64.00
65	2082	65.00
66	2011	66.00
67	1942	67.00
68	1876	68.00
69	1813	68.99
70	1752	69.99
71	1693	71.00
72	1637	71.99
73	1582	73.01
74	1530	74.00
75	1480	75.00
<sup>1</sup> Data from Measurement Specialties™		





## Campbell Scientific Companies

---

**Campbell Scientific, Inc.**

815 West 1800 North  
Logan, Utah 84321  
UNITED STATES

[www.campbellsci.com](http://www.campbellsci.com) • [info@campbellsci.com](mailto:info@campbellsci.com)

**Campbell Scientific Canada Corp.**

14532 – 131 Avenue NW  
Edmonton AB T5L 4X4  
CANADA

[www.campbellsci.ca](http://www.campbellsci.ca) • [dataloggers@campbellsci.ca](mailto:dataloggers@campbellsci.ca)

**Campbell Scientific Africa Pty. Ltd.**

PO Box 2450  
Somerset West 7129  
SOUTH AFRICA

[www.campbellsci.co.za](http://www.campbellsci.co.za) • [cleroux@csafrica.co.za](mailto:cleroux@csafrica.co.za)

**Campbell Scientific Centro Caribe S.A.**

300 N Cementerio, Edificio Breller  
Santo Domingo, Heredia 40305  
COSTA RICA

[www.campbellsci.cc](http://www.campbellsci.cc) • [info@campbellsci.cc](mailto:info@campbellsci.cc)

**Campbell Scientific Southeast Asia Co., Ltd.**

877/22 Nirvana@Work, Rama 9 Road  
Suan Luang Subdistrict, Suan Luang District  
Bangkok 10250  
THAILAND

[www.campbellsci.asia](http://www.campbellsci.asia) • [info@campbellsci.asia](mailto:info@campbellsci.asia)

**Campbell Scientific Ltd.**

Campbell Park  
80 Hathern Road  
Shepshed, Loughborough LE12 9GX  
UNITED KINGDOM

[www.campbellsci.co.uk](http://www.campbellsci.co.uk) • [sales@campbellsci.co.uk](mailto:sales@campbellsci.co.uk)

**Campbell Scientific Australia Pty. Ltd.**

PO Box 8108  
Garbutt Post Shop QLD 4814  
AUSTRALIA

[www.campbellsci.com.au](http://www.campbellsci.com.au) • [info@campbellsci.com.au](mailto:info@campbellsci.com.au)

**Campbell Scientific Ltd.**

3 Avenue de la Division Leclerc  
92160 ANTONY  
FRANCE

[www.campbellsci.fr](http://www.campbellsci.fr) • [info@campbellsci.fr](mailto:info@campbellsci.fr)

**Campbell Scientific (Beijing) Co., Ltd.**

8B16, Floor 8 Tower B, Hanwei Plaza  
7 Guanghua Road  
Chaoyang, Beijing 100004  
P.R. CHINA

[www.campbellsci.com](http://www.campbellsci.com) • [info@campbellsci.com.cn](mailto:info@campbellsci.com.cn)

**Campbell Scientific Ltd.**

Fahrenheitstraße 13  
28359 Bremen  
GERMANY

[www.campbellsci.de](http://www.campbellsci.de) • [info@campbellsci.de](mailto:info@campbellsci.de)

**Campbell Scientific do Brasil Ltda.**

Rua Apinagés, n.br. 2018 – Perdizes  
CEP: 01258-00 – São Paulo – SP  
BRASIL

[www.campbellsci.com.br](http://www.campbellsci.com.br) • [vendas@campbellsci.com.br](mailto:vendas@campbellsci.com.br)

**Campbell Scientific Spain, S. L.**

Avda. Pompeu Fabra 7-9, local 1  
08024 Barcelona  
SPAIN

[www.campbellsci.es](http://www.campbellsci.es) • [info@campbellsci.es](mailto:info@campbellsci.es)

Please visit [www.campbellsci.com](http://www.campbellsci.com) to obtain contact information for your local US or international representative.