

INSTRUCTION MANUAL



CS110 Electric Field Meter

Revision: 4/12



Copyright © 2005-2012
Campbell Scientific, Inc.

WARRANTY AND ASSISTANCE

This equipment is warranted by CAMPBELL SCIENTIFIC (CANADA) CORP. ("CSC") to be free from defects in materials and workmanship under normal use and service for **twelve (12) months** from date of shipment unless specified otherwise. ***** **Batteries are not warranted.** ***** CSC's obligation under this warranty is limited to repairing or replacing (at CSC's option) defective products. The customer shall assume all costs of removing, reinstalling, and shipping defective products to CSC. CSC will return such products by surface carrier prepaid. This warranty shall not apply to any CSC products which have been subjected to modification, misuse, neglect, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied, including warranties of merchantability or fitness for a particular purpose. CSC is not liable for special, indirect, incidental, or consequential damages.

Products may not be returned without prior authorization. To obtain a Return Merchandise Authorization (RMA), contact CAMPBELL SCIENTIFIC (CANADA) CORP., at (780) 454-2505. An RMA number will be issued in order to facilitate Repair Personnel in identifying an instrument upon arrival. Please write this number clearly on the outside of the shipping container. Include description of symptoms and all pertinent details.

CAMPBELL SCIENTIFIC (CANADA) CORP. does not accept collect calls.

Non-warranty products returned for repair should be accompanied by a purchase order to cover repair costs.



CAMPBELL[®]
SCIENTIFIC

Campbell Scientific (Canada) Corp.
11564 149 Street | Edmonton AB T5M 1W7
780.454.2505 | fax 780.454.2655 | campbellsci.ca

PLEASE READ FIRST

About this manual

Please note that this manual was originally produced by Campbell Scientific Inc. (CSI) primarily for the US market. Some spellings, weights and measures may reflect this origin.

Some useful conversion factors:

Area:	1 in ² (square inch) = 645 mm ²
Length:	1 in. (inch) = 25.4 mm 1 ft (foot) = 304.8 mm 1 yard = 0.914 m 1 mile = 1.609 km
Mass:	1 oz. (ounce) = 28.35 g 1 lb (pound weight) = 0.454 kg
Pressure:	1 psi (lb/in ²) = 68.95 mb
Volume:	1 US gallon = 3.785 litres

In addition, part ordering numbers may vary. For example, the CABLE5CBL is a CSI part number and known as a FIN5COND at Campbell Scientific Canada (CSC). CSC Technical Support will be pleased to assist with any questions.

CS110 Table of Contents

PDF viewers: These page numbers refer to the printed version of this document. Use the PDF reader bookmarks tab for links to specific sections.

1. General Description	1
1.1 CS110 Introduction	1
1.2 CR1000 Datalogger	2
1.3 Meteorological Inputs	2
1.4 Communication and Data Storage	2
1.5 Digital I/O	3
1.6 Self-Check Features	3
2. CS110 Specifications	4
3. CS110 Measurement Details	7
4. Site Requirements and Recommendations	9
4.1 Power Requirements	9
4.2 Campbell Scientific, Inc. Power Supplies	10
4.3 Communication Options	10
4.4 Site Recommendations	11
5. Factory Calibration and Site Correction	11
5.1 Factory Calibration	11
5.2 Site Correction	14
6. Lightning Warning	19
7. CRBasic Programming	21
8. CS110 Measurement Instructions	25
8.1 CR1000 Measurement Overview	25
8.2 Measuring Electric Field	27
8.3 Measuring Electric Field Change	27
8.4 Measuring Solar Radiation or Barometric Pressure	27
8.5 Measuring Air Temperature and Relative Humidity	28
8.6 Measuring Wind Speed and Direction	28
8.7 Measuring Rainfall	29
8.8 Measuring Internal Case Humidity	29
9. PC Software	29
9.1 Quick Start	29

10. Maintenance	33
10.1 Checking Site Ground Integrity	33
10.2 Corrosion and Rust Inhibitors	33
10.3 Self-Check Features	35
10.4 Cleaning the CS110 Electrode Head	36
10.5 Changing Desiccant	37
10.6 Checking Shutter/Encoder Alignment	39
10.7 Re-Calibration	40
 11. References	 40
 Appendices	
 A. CS110 Measurement Status Codes	 A-1
 B. CS110 Accessories	 B-1
B.1 Zero Field Cover Plate	B-1
B.2 Upward-Facing Site Calibration Kit	B-1
B.3 CR1000 Keyboard Display	B-1
B.4 Miscellaneous Peripheral Modules	B-1
 C. CS110 Connector Pin-outs	 C-1
 D. Servicing the CS110	 D-1
D.1 Lid Gasket	D-1
D.2 Changing Out the CR1000	D-1
D.3 Changing Out Motor Assembly	D-2
D.4 Changing Out the CS110 Panel Board Assembly	D-2
D.5 Shutter/Encoder Alignment	D-3
D.6 Motor O-ring Seal	D-6
 E. CS110 as a Slow Antenna	 E-1
E.1 Response of the CS110 Slow Antenna in the Frequency Domain	E-1
E.2 Response of the CS110 Slow Antenna in the Time Domain	E-3
E.3 Programming	E-5
E.4 Calibration	E-6
 F. Example CRBasic Programs	 F-1
 G. CS110 2 Meter CM10 Tripod Site	 G-1

H. Tripod CS110 and StrikeGuard..... H-1

H.1 Tripod CS110 and StrikeGuard H-1
 H.1.1 Installation of the Tripod CS110 and StrikeGuard site H-2
 H.1.2 Determination of Csite H-7

Figures

1. CS110 Electric Field Meter 1
 2. Charge amplifier circuitry of reciprocating electric field meter 7
 3. Charge amplifier output during an electric field measurement cycle 8
 4. CS110 average current consumption versus measurement interval 10
 5. Parallel-plate electric field meter calibration chamber 12
 6. Factory calibration data for CS110 SN: 1026 13
 7. NIST calibration certificate 14
 8. CS110 2 Meter CM10 Tripod Site 15
 9. Campbell Scientific, Inc. electric field meter site correction facility 16
 10. CS110 attached to upward-facing flush-mounted plate for site correction 17
 11. Site correction data for CS110 2 Meter CM10 Tripod Site 18
 12. Electric field measured with CS110 during local thunderstorm 20
 13. CS110 stator, shutter and sense electrode 36
 14. Inside of CS110 case illustrating bracket for holding desiccant 38
 D-1. Exploded View of CS110 Electric Field Meter D-1
 D-2. CS110 Motor Assembly D-5
 E-1. CS110 slow antenna frequency response E-2
 E-2. KSC electric field and CS110 slow antenna data E-3
 E-3. KSC electric field change and CS110 slow antenna data E-4
 G-1. CS110 2 Meter CM10 Tripod Site G-1
 G-2. CS110 on CM10 Tripod Mast G-3
 G-3. Earth Grounding G-4
 G-4. Determination of Csite G-5
 H-1. Tripod CS110 and StrikeGuard H-1
 H-2. CS110 and StrikeGuard on Tripod Mast H-3
 H-3. Grounding the CS110 Grounding Strap H-4
 H-4. Grounding the Tripod and Battery H-5
 H-5. Connections for Combined System H-6
 H-6. Determination of Csite H-7

CS110 Electric Field Meter

1. General Description

1.1 CS110 Introduction

Atmospheric electric fields have been measured for decades by electric field meters nicknamed “field mills”. Traditional field mills employ a spinning metal rotor (vane) electrically connected to Earth ground, placed between the external field and stationary metal sense electrodes. The grounded spinning rotor alternately shields and exposes the sense electrodes from the electric field to be measured, resulting in a modulation of the induced charge on the sense electrodes. Typically, a pair of charge amplifiers converts the modulated charge into AC voltages that are synchronously rectified and filtered to form a low-frequency voltage proportional to the low-frequency (≤ 10 Hz) electric field.

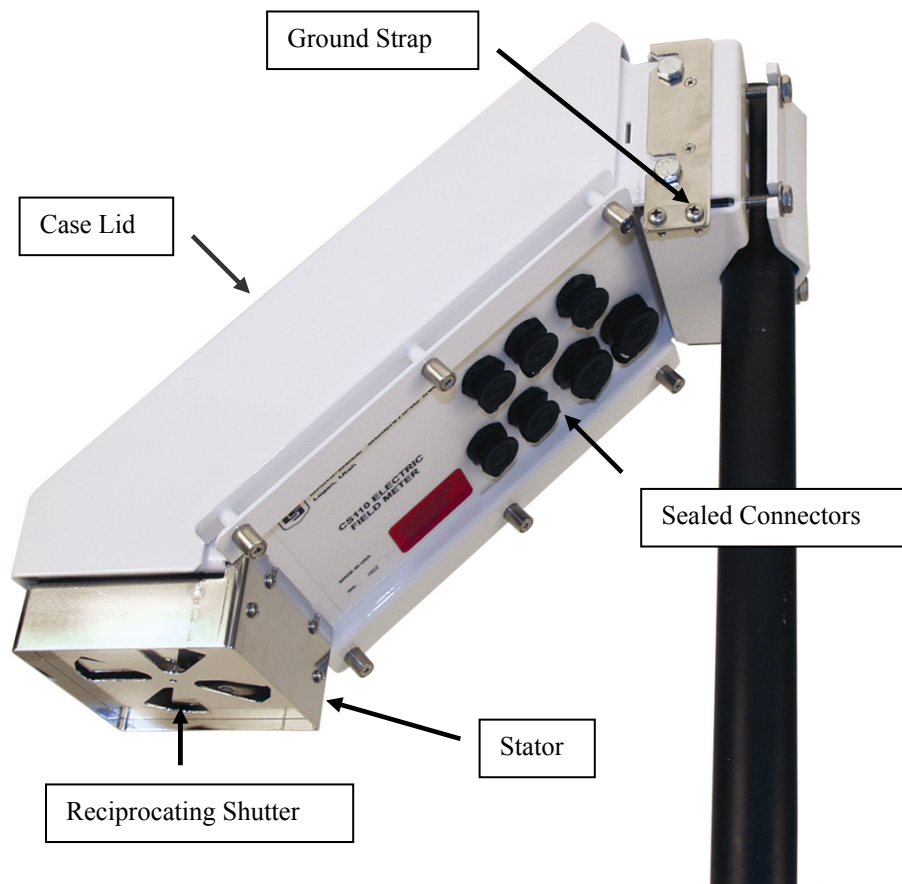


FIGURE 1. CS110 Electric Field Meter

Unlike traditional rotating vane field mills, the CS110 uses a reciprocating shutter. A stepper motor opens and then closes the reciprocating shutter by 45° during measurements. The reciprocating shutter is electrically connected to ground potential by a flexible stainless-steel strap operated below its fatigue limit, resulting in an ultra-reliable electrical ground connection. The CS110 offers improved dc error performance, as compared with traditional rotating vane field mills, by utilizing a zero field (closed shutter) reference for each measurement. Power consumption is also reduced (< 1 Watt for 1 measurement per second) in the CS110 by de-energizing the motor coils in between measurements.

1.2 CR1000 Datalogger

The CS110 contains an embedded CR1000 datalogger, which provides measurement and control functions, data processing and storage, a user interface language (CRBasic™), and flexible communications options. LoggerNet™ PC software (purchased separately) provides versatile networking and data collection capabilities. For more details on the CR1000 datalogger see the CR1000 Measurement and Control System Operator's Manual.

1.3 Meteorological Inputs

The CS110 interfaces to various meteorological sensors resulting in an automated weather station that includes atmospheric electric field. Wind speed and direction, air temperature and relative humidity, rainfall, solar radiation or barometric pressure sensors interface directly to the CS110. Measurement details of the various sensors are given in section 7.

1.4 Communication and Data Storage

The circular RS-232 connector on the underside of the CS110 can be used to interface directly to RS-232 devices (DTE or DCE), utilizing the CS110 RS-232 cable (CS110CBL1-L).

The circular CS I/O connector on the underside of the CS110 can be used to interface directly to various Campbell Scientific, Inc. peripherals, utilizing the CS110 CS I/O cable (CS110CBL2-L). Examples of CS I/O peripherals include the CR1000 Keyboard Display and the COM220 phone modem.

The DB9 end of CS110 RS-232 cable and CS110 CS I/O cable won't fit through the conduit used on some enclosures, whereas the smaller circular end that connects to the CS110 will.

The embedded CR1000 will have either 2 MB (PN: 18292) or 4 MB (PN: 18293) of battery-backed SRAM and 16K Flash EEPROM. The operating system and user programs are stored in Flash EEPROM. Memory not used by the operating system and user program is available for data storage. The size of available memory can be seen in the Status Table discussed in Appendix B of the CR1000 manual.

1.5 Digital I/O

Three general purpose 0 to 5 V digital I/O lines are available on the CS110 Power cable (CS110CBL3-L) that attaches to the circular power connector on the underside of the CS110. The blue, yellow, and green wires connect to control ports C1, C2, and C3 respectively. Using CRBasic, these digital I/O lines can be used to conditionally turn on alarms, provide an interrupt or pulsed signal to be measured by the CS110, or as a serial communication port.

1.6 Self-Check Features

The CS110 has been designed to provide reliable electric field measurements and to minimize and simplify maintenance. The CS110 incorporates extensive self-checking for each measurement in an effort to identify measurement problems and reduce or eliminate scheduled maintenance. The status code returned from each electric field measurement reports on instrument health along with any measurement problems as described in Appendix A.

For example, insulator leakage current is measured during each electric field measurement, indicating the cleanliness of electrode insulators. A leakage current compensation circuit for the charge amplifier input is incorporated in the CS110 to minimize the effects of insulator leakage current on measured results (Patent pending). A status code indicating excessive leakage current is returned if the measured input leakage current exceeds the compensation range due to insulator cleanliness problems.

A relative humidity sensor is included inside the CS110 case to provide information on when case desiccant should be changed. The CS110 also provides measurement of the battery input voltage in order to monitor the input power to the instrument. Section 7 discusses CS110 electric field measurement details. CS110 maintenance details are discussed in Section 10.

2. CS110 Specifications

Electric Field Measurement Performance:

<i>Parallel-Plate Configuration</i>			
<i>Accuracy</i>	±1% of reading + 60 V m ⁻¹ offset ¹		
<i>Measurement Range</i> ³ (V m ⁻¹)	<i>Resolution</i> (V m ⁻¹)	<i>Sensitivity</i> (μV/V m ⁻¹) ¹	<i>Noise</i> (V m ⁻¹) <u>RMS</u>
±(0 to 21,000)	3	12	4.0
±(21,000 to 212,000)	30	118	18.0
<i>2 m CM10 Tripod Configuration</i> ²			
<i>Accuracy</i>	±5% of reading + 8 V m ⁻¹ offset ¹		
<i>Measurement Range</i> ³ (V m ⁻¹)	<i>Resolution</i> (V m ⁻¹)	<i>Sensitivity</i> (μV/V m ⁻¹) ¹	<i>Noise</i> (V m ⁻¹) <u>RMS</u>
±(0 to 2,200)	0.32	1.2	0.42
±(2,200 to 22,300)	3.2	13	1.9
<p>¹Typical offset for clean electrodes is ≤ 30 V m⁻¹ for the parallel-plate configuration, which is reduced by the field enhancement factor for typical inverted and elevated mounting configurations.</p> <p>²Field enhancement due to typical inverted and elevated mounting requires additional site correction, estimated at ±5% accuracy when done in appropriate high field conditions. Practical outdoor CS110 electric field measurement accuracy is estimated at ±5% of reading + 8 V m⁻¹ for the CS110 2 Meter CM10 Tripod Site.</p> <p>³The CS110 incorporates automatic gain ranging between two input ranges. The measurement is first tried on the lowest input range. If the signal is too large for the lowest range, the larger range is used.</p>			

Standard Mounting: 2 m height on a CM10 tripod mast

Site Correction: Site correction factors available for several standard mounting configurations

Sample (Measurement) Rate:	Programmable sample rate up to 5 samples per second, variable sample rates possible. Variable example: sample every 10 seconds until field exceeds threshold then sample once a second until field returns to normal.
Power Requirements:	11 to 16 Vdc; peak-current demand is 750 mA during motor operation. 7 mA @ 12 V = 0.08 W average power consumption at 1 sample per 10 seconds 60 mA @ 12 V = 0.7 W average power consumption at 1 sample per second 120 mA @ 12 V = 1.4 W average power consumption at 2 samples per second 300 mA @ 12 V = 3.6 W average power consumption at 5 samples per second
Communication:	1 RS-232 port; 1 CS I/O port used to interface with our peripherals such as a COM320 Voice Modem; digital control ports 1, 2, and 3 for alarm, SDI-12 communications, or asynchronous communications
Baud Rates:	Selectable from 300 to 115,200 bps
ASCII Protocol:	One start bit, one stop bit, eight data bits, no parity
Lightning Protection:	Multi-stage transient protection on all external interfaces
CE Compliance:	Standards to which conformity is declared—BS EN61326:2002
Connectors/ Compatible Sensors:	<i>Connector Label Compatible Sensors¹</i>
Temp/RH:	HC2S3-L, HMP60-L (choose the -C cable termination option for these sensors)
Wind:	05103-LC, 05106-LC, 05305-LC, 034B-LC, 03001-LC
Solar:	LI200X-LC pyranometer, CS100 barometer or CS106 barometer (the barometer attaches to the CS110 via the 17640 cable; they must be housed in a separate enclosure such as the ENC100)
Rain:	CS700-LC, TB4-LC, TE525-LC, TE525WS-LC, TE525MM-LC
	¹ One sensor per connector
Programmability:	CRBasic™ programming allows the selection of sample rate, data processing and storage options and setting output ports based on alarm conditions. LoggerNet™ includes the CRBasic editor and compiler.

Rugged Construction:	Ultra-reliable metallic ground connection to reciprocating shutter (no wiping contact), brushless stepper motor, powder-coated aluminum case, Teflon insulators, and electro-polished 316L stainless steel used for corrosion protection of critical exposed metallic parts
Easy Maintenance:	The stator is easily removed for cleaning (proper cleaning does not invalidate calibration). Instrument self-checking allows maintenance to be performed on an as needed basis. The self-checking also monitors internal humidity, insulator cleanliness, and power supply voltage, and verifies that CS110 components such as the charge amplifier and shutter open/close are functioning properly.
Operating Temperature Range:	-25° to 50°C standard, -40° to +85°C optional
RH Range:	0 to 100% RH
Dimensions:	15.2 x 15.2 x 43.2 cm (6 x 6 x 17 in)
Mounting:	Vertical pipe 1.91 to 6.35 cm OD (0.75 to 2.5 in)
Weight:	4 kg (9 lb)

3. CS110 Measurement Details

The charge amplifier circuitry of the reciprocating electric field meter is depicted in Figure 2. Induced charge on the sense electrode results in the operational amplifier placing charge on the feedback capacitor C in order to restore the sense electrode to virtual ground.

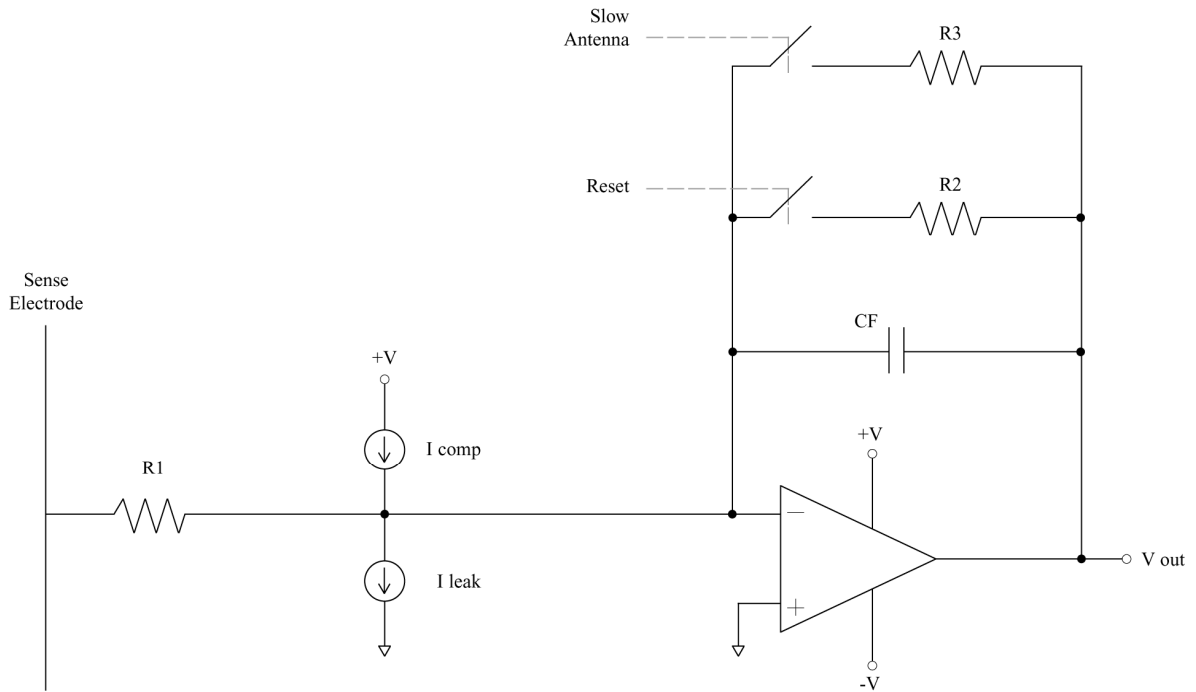


FIGURE 2. Charge amplifier circuitry of reciprocating electric field meter

The charge amplifier output during a measurement cycle of the reciprocating electric field meter is illustrated in Figure 3.

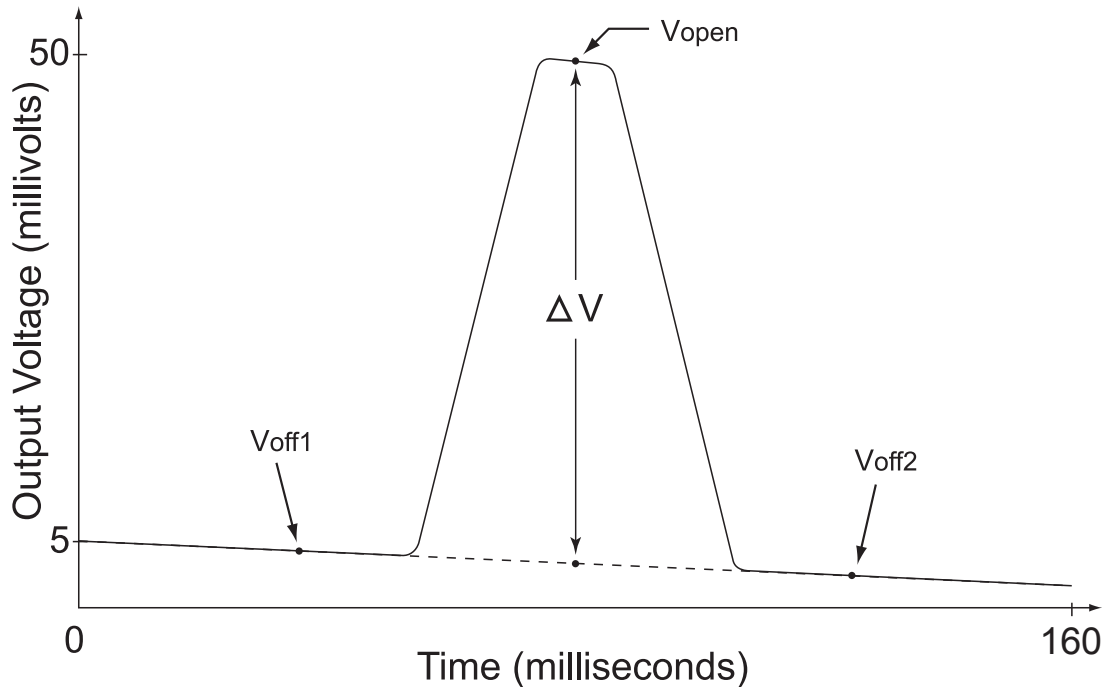


FIGURE 3. Charge amplifier output during an electric field measurement cycle

Offset voltages V_{off1} and V_{off2} are zero field reference measurements made when the shutter is closed, and utilized to accurately estimate voltage ΔV when the shutter is completely open. Electronic offset voltages, surface potentials between various metallic parts and leakage currents on the charge amplifier input result in non-zero values of V_{off1} and V_{off2} . An electronic reset of the charge amplifier is performed prior to the measure of V_{off1} to keep the charge amplifier output near zero volts when the shutter closed. The measured electric field E , as determined from the charge amplifier output is as follows:

$$E = k \cdot \Delta V = k \cdot [V_{open} - (V_{off1} + V_{off2})/2] \quad (\text{eq. 1})$$

Where k is a constant determined by electrode geometry and electronic gain.

The resulting algorithm effectively eliminates measurement error sources that vary slowly with respect to the time between zero field reference measurements, which is approximately 140 ms. Measurement noise due to 50 or 60 Hz AC power can be suppressed by utilizing the 50 Hz or 60 Hz noise rejection measurement capability of the datalogger.

Current source I_{leak} in Figure 2 represents leakage currents across the Teflon insulators supporting the sense electrode, along with the input bias current of the operational amplifier. Deleterious effects of I_{leak} are compensated for in the determination of ΔV as given in (eq. 1). However, it is desirable to minimize the difference between V_{off1} and V_{off2} in order to preserve dynamic range for large magnitude V_{open} voltages. Hence a leakage-current compensation circuit is utilized to generate the current I_{comp} , illustrated in Figure 2, such that $I_{comp} = I_{leak}$. The leakage-current compensation algorithm determines I_{comp} for the present measurement based on I_{leak} from the previous measurement, which is determined as follows:

$$I_{\text{leak}} = C_f(V_{\text{off1}} - V_{\text{off2}})/\Delta T + I_{\text{comp}} \quad (\text{eq. 2})$$

Where C_f is the value of feedback capacitor used in the charge amplifier, and I_{comp} is the leakage current compensation value implemented during the measurement.

This charge amplifier input leakage current increases with degradation of insulation of the sense electrode insulators due to moisture or other surface contamination. Consequently, the measurement and reporting of I_{leak} is useful in determining if or when insulators should be cleaned.

The reciprocating motion of the CS110 electric field meter is limited to approximately 5 Hz, which is adequate for lightning hazard warning, where 1 minute averaged data is often used. For applications desiring > 5 Hz, the CS110 reciprocating electric field meter can be configured as a slow antenna (MacGorman and Rust 1998). The shutter would typically be left open indefinitely in slow antenna mode and resistor R3, depicted in Figure 2, is switched in parallel with C_f providing a 66 ms decay time constant for the charge amplifier. In the slow antenna mode, the charge amplifier has a high-pass filter frequency response with the lower cutoff frequency defined as $f_{3\text{dB}} = (2 \cdot \pi \cdot R \cdot C)^{-1} = 2.4$ Hz. In this mode the instrument is a field change meter and the charge amplifier output can be sampled by the datalogger as fast as every 20 ms (50 Hz), using 250 μs integration durations for the analog integrator. Voltage measurements using the 250 μs integration duration for an analog integrator, result in an upper 3 dB bandwidth of 1.8 kHz. Detailed information regarding the slow antenna mode of the CS110 is given in Appendix E and Section 8.3.

4. Site Requirements and Recommendations

4.1 Power Requirements

Field mills typically consume many watts of power because their motors are operated continuously. In the reciprocating approach, the stepper motor is powered off much of the time, resulting in low power consumption. The current required by the CS110 powered from 12 V DC is shown in Figure 4. As depicted in the figure, the average electric field meter current is a function of the desired measurement rate, which is user-controlled by means of the datalogger program, making economical remote solar power feasible. Variable sample rates based on measured results can also be implemented to conserve power in solar powered applications. For example, the datalogger can be programmed to measure electric field at a 10-second rate during fair weather conditions, and then automatically switch to 1-second measurements during threatening conditions. An example variable sample rate program is given in Appendix F. Figure 4 does not include the current required for peripheral devices necessary to communicate with the CS110 site. Like the stepper motor, communication devices that are turned off when not needed, can offer low average power consumption.

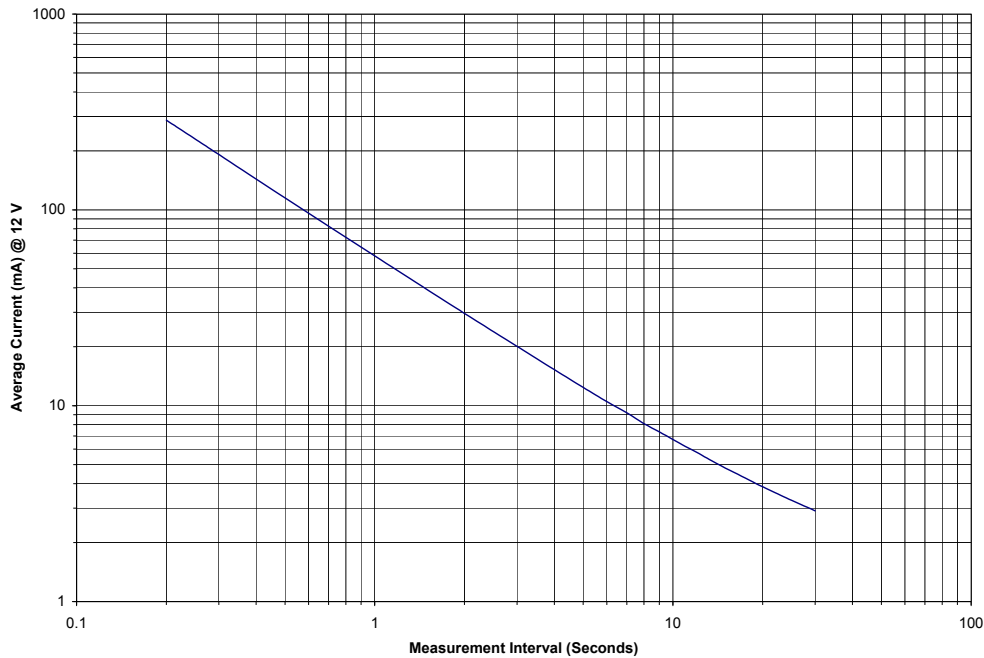


FIGURE 4. CS110 average current consumption versus measurement interval

The CS110 requires 11 V to 16 Vdc with a peak current demand of 750 mA during motor operation. The CS110 Power Cable (pn 16965) is used to connect the dc power supply to the CS110. **The recommended maximum length on the CS110 Power Cable (CS110CBL3-L) is 50 feet.** The CS110 is protected against accidental reversal of the positive and ground leads from the dc power supply. Transient protection is also included on the power supply inputs. DC input voltages in excess of 18 V may damage the CS110.

4.2 Campbell Scientific, Inc. Power Supplies

The PS100 provides a 12 Vdc, 7.0 Ahr rechargeable power supply for the CS110 and peripherals. The CH100 is a charging regulator for 12 V rechargeable batteries that is commonly used with the larger 12 amp hour (BP12) and 24 amp hour (BP24) Battery Packs. The rechargeable battery can be trickle-charged from an ac power wall charger. The PN: 9591 wall charger accepts 110 Vac while the PN: 14014 accepts 90 to 264 Vac. Charging power can also come from a 17 – 28 VDC input such as a solar panel. Depending on power requirements, 10 watt or 20 watt solar panels (SP10 or SP20) are available.

4.3 Communication Options

The circular RS-232 connector on the underside of the CS110 can be used to interface directly to RS-232 devices (DB-9), utilizing the CS110 RS-232 cable (CS110CBL1-L).

The circular CS I/O connector on the underside of the CS110 can be used to interface directly to various Campbell Scientific, Inc. peripherals, utilizing the

CS110 CS I/O cable (CS110CBL2-L). Examples of CS I/O peripherals include the CR1000 Keyboard Display and the COM220 phone modem.

The CS110 also offers SDI-12 communication or SDM (Synchronous Device for Measurement) control capability utilizing the CR1000 control ports available through the CS110 POWER CABLE (CS110CBL3-L).

4.4 Site Recommendations

Many factors can distort and/or change the electric field at a given sight. For example, vegetation growth can reduce the effective height of an elevated instrument above the ground and can create unwanted space-charge due to corona discharge. Gravel rings or concrete pads around a given site are recommended to prevent changes in effective instrument height due to vegetation growth. Electric field meters used for lightning warning at Kennedy Space Center use a 25-foot radius gravel ring around each electric field meter [LPLWS].

Animals and people within the vicinity of an electric field meter can significantly alter the measurements. Fencing off a given site may be best for some applications. However, installing a **small** metal fence around an electric field meter site may result in corruption of measurements at large electric fields because of corona discharge from sharp metal points on the fence.

Aerosols, dust, and automobile exhaust should be considered when selecting an electric field meter site, as they can affect the local electric field.

In theory, the effects of tall nearby objects can be accounted for in site correction. Yet, because of possible corona current along with general field distortion, it is recommended that electric field meter sites should not be located near tall objects. Kennedy Space Center site requirements stipulate having no objects protruding higher than 18° above the horizon, as seen from the ground at the electric field meter location [LPLWS]. Roof mounted electric field measurements are practical if a site correction can be done to account for field distortions.

Also a good Earth ground connection to the CS110 and associated mounting hardware is necessary to make a given site appear as a vertical extension of the Earth ground. It is recommended that the integrity of this Earth Ground connection be checked periodically by verifying that the resistance of the stator to Earth Ground rod is $<1 \Omega$.

Although the list of factors that can impair electric field measurements is long, experience has shown that useful electric field measurements can be made by paying careful attention to the above mentioned details.

5. Factory Calibration and Site Correction

5.1 Factory Calibration

Electric field meters are typically factory calibrated using a parallel plate method, where a uniform electric field is developed by applying a known voltage between parallel conductive plates. The large hexagonal parallel plate electric field calibrator illustrated in Figure 5 is used for factory calibration of the CS110 Electric Field Meter. The large physical size was incorporated to

minimize non-ideal fringing effects. Sharp corners were avoided in order to prevent corona discharge. All metal parts of the calibrator are manufactured from stainless steel, and the inside surfaces are polished to reduce the surface charges in order to provide a stable zero electric field. All outer surfaces are electrically connected and tied to Earth ground while the insulated inner plate is driven by a high voltage amplifier. The high-voltage amplifier is calibrated out-of-house yearly against a reference that is traceable to the National Institute of Standards and Technology (NIST).

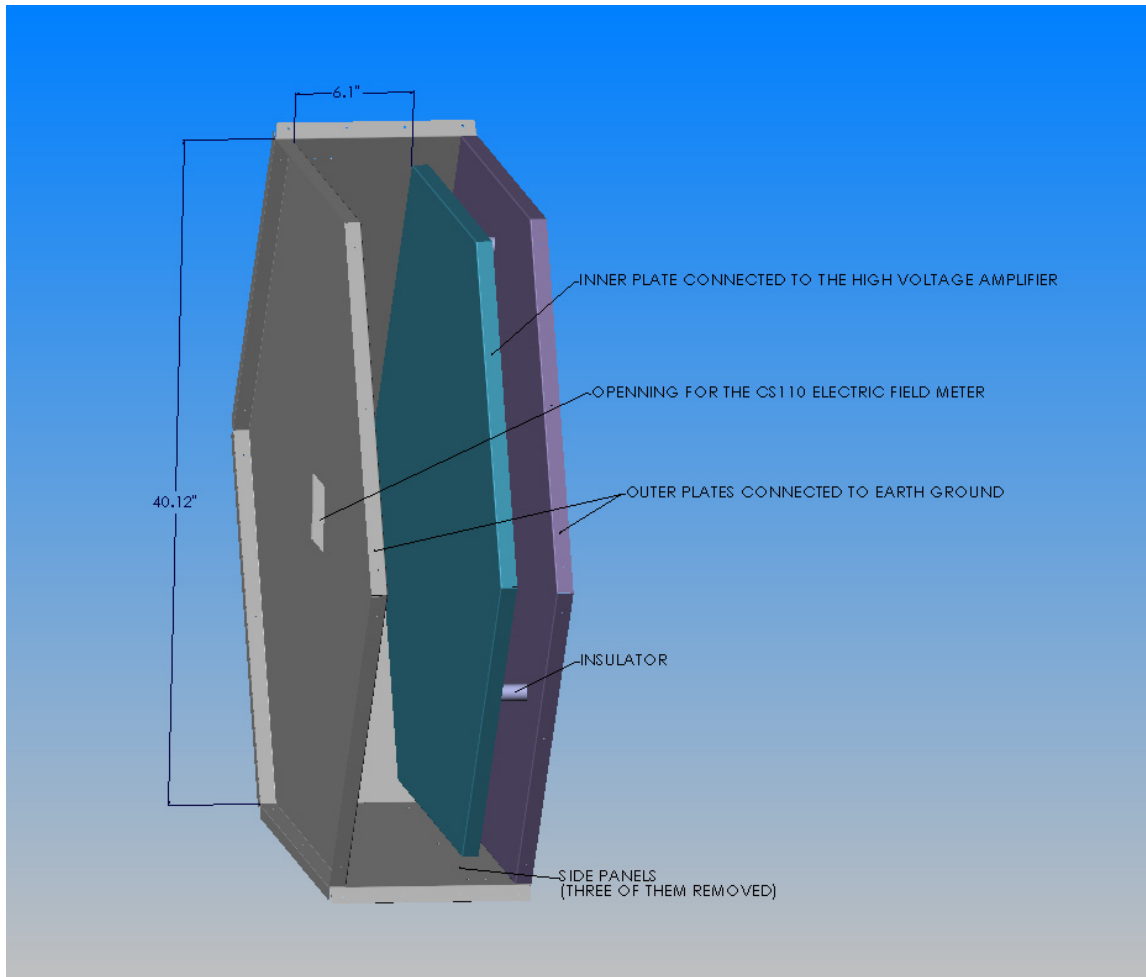


FIGURE 5. Parallel-plate electric field meter calibration chamber

Each CS110 is factory calibrated in the parallel plate calibration fixture depicted in Figure 5. A linear fit of the calibration data results in a calibration equation in slope-intercept form expressed as

$$E = M_{\text{parallel_plate}} \cdot V + O_{\text{parallel_plate}} \quad (\text{eq. 3}).$$

The multiplier $M_{\text{parallel_plate}}$ is a function of the CS110 electrode dimensions and the feedback capacitor in the charge amplifier. The offset term $O_{\text{parallel_plate}}$ is due to unwanted surface charges residing on non-conductive deposits on the electrodes. The electric field offset of an instrument varies over time because

of variations in surface cleanliness along with charging and discharging processes. Polished 316-L stainless-steel is used for critical electrode surfaces on the CS110 to minimize unwanted surface charges. CS110s with clean electrodes have been found to display electric field offsets $< |30 \text{ V/m}|$, which has negligible effect on the determination of $M_{\text{parallel_plate}}$ because of the $\pm 15 \text{ kV/m}$ range of electric fields used during factory calibration. Neglecting $O_{\text{parallel_plate}}$ results in the simplified parallel-plate calibration equation

$$E = M_{\text{parallel_plate}} \cdot V \tag{eq. 4}$$

The estimated measurement accuracy of $M_{\text{parallel_plate}}$ for the CS110 calibrated in the parallel plate electric field calibrator illustrated in Figure 5 is $\pm 1 \%$. The electric field offset of the CS110 can be measured by covering the stator with a clean Zero Electric Field Cover (PN: 17642). If the resulting zero field reading with the zero field cover exceeds an absolute value of 60 V/m then cleaning of electrodes in the CS110 is suggested. The factory calibration data for a typical CS110 factory calibration and resulting determination of $M_{\text{parallel_plate}} = 84.32 \text{ V/m}\cdot\text{mV}$ (Volts/meter-millivolt) is illustrated in Figure 6.

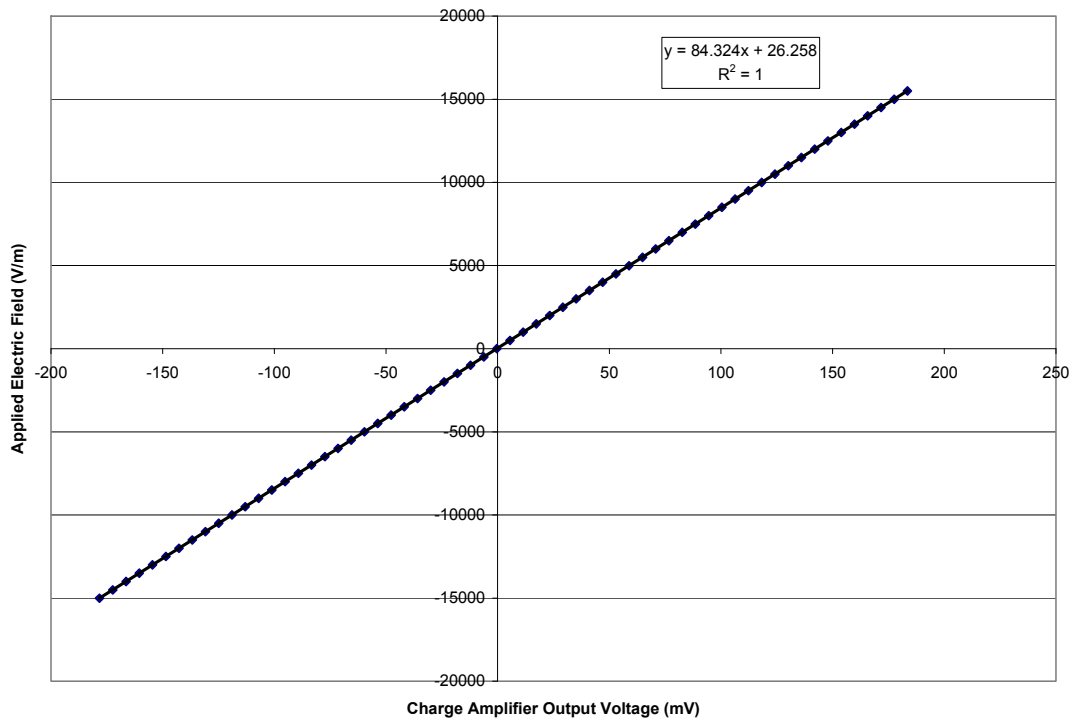


FIGURE 6. Factory calibration data for CS110 SN: 1026



CAMPBELL SCIENTIFIC, INC.

815 W. 1800N. Logan, Utah 84321-1784 (435) 753-2342 FAX (435) 750-9540 www.campbellsci.com

Certificate of Calibration

Model: CS110 - L
CS110 Serial Number: 1172
CR1000 Serial Number: 25836
Calibration Procedure: TST16058B 04
Instrument Calibration Condition: In Tolerance
Calibration Date: 7/14/2009

Calibration Standards Used:

Model: Trek 609E-6-L-CE
 S/N: 212
 Cal. Due Date: 3/16/2010
 NIST Reference: 263994

Instrument Data: Multiplier = 85.75 R Squared Value = 1

Environment Temperature (C) 25 Relative Humidity (%) 10.5

Calibration By: W. Iverson
 W. Iverson

Campbell Scientific, Inc. certifies the above instrument meets or exceeds published specifications and has been calibrated using a Voltage Standard whose gain accuracy is traceable to the National Institute of Standards and Technology. Electrostatic field measurements are not NIST Traceable. Refer to the CS110 Operators manual for more information. The policies and procedures at this calibration facility comply with ISO-9001.

FIGURE 7. NIST calibration certificate

NOTE

Careful removal and replacement of the stator on the CS110 does not invalidate the factory derived $M_{\text{parallel_plate}}$ of a given unit. However, switching stators with another unit or accidentally bending the stator, shutter or sense electrodes invalidates the factory parallel-plate calibration because of possible electrode dimensional changes.

5.2 Site Correction

As previously mentioned, each CS110 is factory calibrated in a parallel plate calibration fixture resulting in calibration equation 4. However, when monitoring the Earth's electric field, equation 4 is valid only if the instrument aperture is mounted flush with the Earth's surface and upward-facing. Yet for permanent outdoor measurements of electric field, a flush-mounted and upward-facing orientation is problematic because of dirt, bird droppings, rain, etc., collecting on the sense electrodes and fouling the measurement.

Consequently, a downward facing and elevated configuration as illustrated in Figure 8 is recommended for long-term field applications.



FIGURE 8. CS110 2 Meter CM10 Tripod Site

Inverting the CS110 reduces the effective gain while elevating its height above ground enhances the gain, with respect to an ideal upward-facing flush-mounted geometry. It should be mentioned that this gain enhancement reduces the effect of unwanted electrical field offsets. A site correction factor C_{site} is necessary to correct $M_{\text{parallel_plate}}$ for non flush-mounted configurations [McGorman and Rust]. The corrected multiplier $M_{\text{corrected}}$ becomes as follows:

$$M_{\text{corrected}} = C_{\text{site}} \cdot M_{\text{parallel_plate}} \quad (\text{Eq. 5}).$$

In equation 5, $M_{\text{parallel_plate}}$ is unique for each CS110, yet independent of a given site, whereas C_{site} is unique for each given site, yet independent of the particular CS110 used at the site. C_{site} is typically determined by using a flush-mounted upward-facing unit in the vicinity of the site needing correction. Campbell Scientific, Inc. developed the site correction facility illustrated in Figure 9 to determine C_{site} for various site configurations.



FIGURE 9. Campbell Scientific, Inc. electric field meter site correction facility

An upward-facing calibration kit (PN: 17579) was developed to hold the CS110 in a flush-mounted upward-facing position, as illustrated in Figure 10.



FIGURE 10. CS110 attached to upward-facing flush-mounted plate for site correction

NOTE


Both the upward-facing and the inverted and elevated unit need to be electrically connected to Earth potential. This can best be accomplished by a grounding rod and wire connected to ground lugs provided on both the upward-facing plate and on the mounting bracket on the standard CS110.

Ideally, site correction should be done in the absence of precipitation, and during the presence of slowly varying electric fields of bipolar polarity and magnitudes large enough to make instrument offset errors negligible. These conditions may be infrequent in practice, making site correction using a flush-mounted upward-facing unit somewhat challenging. Falling precipitation along with blowing dirt can result in questionable measurements by an exposed, upward-facing unit. Cleaning of the electrodes of an upward-facing unit is recommended after it has been exposed to blowing dust and/or falling precipitation. The measurement of meteorological parameters such as rainfall, along with the averaging and data storage capability of the CS110 can be

utilized to autonomously measure, process and store data to aid in site correction.

Campbell Scientific, Inc. has performed a site correction on the CS110 2 Meter CM10 Tripod Site described in Appendix G. The collected data between the upward-facing unit and a downward facing CS110 2 Meter CM10 Tripod Site is illustrated in Fig 10. A best-fit line computed from the data resulted in $C_{site} = 0.105 \pm 4\%$, which is valid for users at other sites who use the same site dimensions on level terrain clear of vegetation. Dimensional details of the 2 meter standard meteorological site are described in Appendix F.

**10/02/05 Site Correction of CS110 2 Meter CM10 Tripod Site
Results indicate Csite = 0.105.**

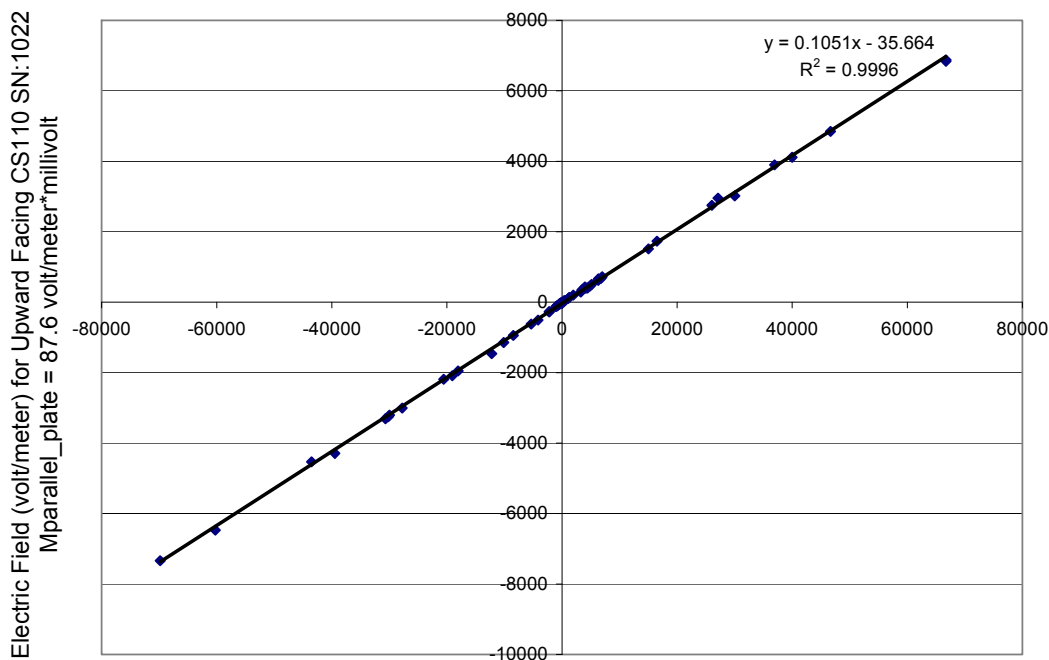

Uncorrected (Csite = 1) Electric Field (volt/meter) for 2 Meter Mounted CS110 on CM10 Tripod. SN: 1023 Mparallel_Plate = 81.77 volt/meter*millivolt

FIGURE 11. Site correction data for CS110 2 Meter CM10 Tripod Site

The user is responsible for determining if a CS110 site is representative of the CS110 2 Meter CM10 Tripod Site, and if not, for determining the appropriate site correction.

The atmospheric electric field at the Earth’s surface during fair weather conditions is on the order of -100 V/m; the negative sign indicating that the electrostatic force on a positive charge is directed downward to the Earth’s surface [McGorman and Rust],[Rakov and Uman]. Ballpark site corrections are sometimes computed in fair weather conditions by assuming a -100 V/m fair weather field. The accuracy of a fair weather site correction is questionable because local conditions may result in a fair weather field significantly different ($>100\%$) from -100 V/m. Also, the unknown electric field offset may be significant when calibrating at -100 V/m. This offset can be measured by

covering the stator with a clean Zero Electric Field Cover (PN: 17642). Fair weather field site correction is not recommended for lightning warning applications because of the relatively poor accuracy in determining Csite.

6. Lightning Warning

Lightning warning devices fall into two classes: lightning detectors and electric field monitors. Stand-alone lightning detectors provide warning based on nearby discharges, but give no warning until a detectable discharge occurs. Electric field monitors measure the atmospheric electric field, indicating the presence of nearby electrified clouds capable of producing lightning discharges. Consequently, electric field monitors can give warning at the beginning of storms prior to hazardous discharges. Both lightning detectors and electric field monitors are employed in high-risk applications.

Lightning safety guidelines based on human observations exist and should not be ignored simply because of the presence of sensitive electronic instrumentation. The NOAA 30/30 rule suggests seeking shelter if thunder is heard within 30 seconds of a lightning flash (approximately 6 miles), and remaining in a sheltered area for 30 minutes after the last lightning or thunder before resuming outdoor activities [NOAA].

It should be noted that **no method of lightning warning completely eliminates the risks associated with lightning.** As mentioned, lightning detectors give no warning until a detectable discharge has occurred. Atmospheric electric field yields warning prior to the “first strike” for storms developing overhead, along with some indication of the end of a thunderstorm. Yet there are occurrences of cloud-to-ground lightning discharges striking the ground several miles away from the electrified cloud where the discharge initiated [NOAA]. Electric field monitors may give no practical warning in these instances because the electric field in the vicinity of the strike point may not indicate hazardous levels until milliseconds before the strike. Consequently, **while lightning warning systems can greatly reduce the probability of death or injury from lightning discharges, they cannot reduce this probability to zero.**

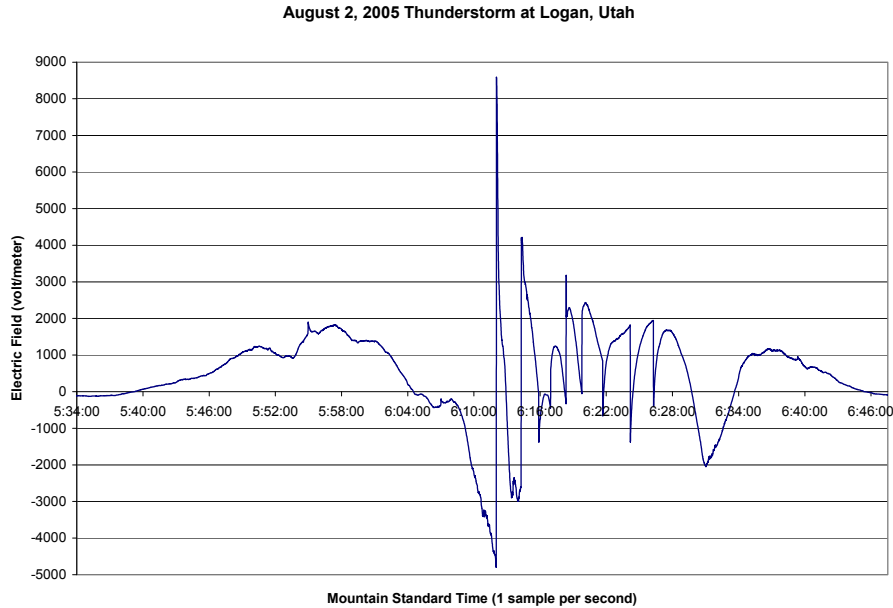


FIGURE 12. Electric field measured with CS110 during local thunderstorm

Figure 12 illustrates the atmospheric electric field monitored by a CS110 during a local thunderstorm. As illustrated in Figure 12, the atmospheric electric field changes dramatically from fair weather conditions (≈ -100 V/m) during the course of this thunderstorm. The abrupt electric field change observed at approximately 6:12 am was due to a hazardous cloud-to-ground lightning discharge. A lightning hazard warning algorithm would ideally issue an alarm, or perhaps various caution/alarm levels, during the critical front-end portion of the storm illustrated in Figure 12, as the electric field is seen to deviate from a typical fair weather field and approach levels capable of producing hazardous lightning discharges. There is no universal hazard alarm level based on atmospheric electric field, although two levels that have been used are $\geq |1000$ V/m [LPLWS] and $\geq |2000$ V/m [NAVSEA]. Obviously the lower the level used the more risk reduction available, at the expense of increased down time for operations suspended for lightning hazard warning. **Campbell Scientific, Inc. is not liable for the reliability and performance of the warning algorithms implemented by users of our equipment. While lightning warning systems can greatly reduce the probability of death or injury from lightning discharges, they cannot reduce this probability to zero.**

As previously mentioned, both lightning detection and electric field monitoring are used for lightning warning systems in high-risk applications. Lightning detectors with serial digital outputs can be interfaced to the CS110 resulting in both lightning detection and electric field monitoring for a given site. The CS I/O port, along with the three general purpose 0 to 5 V digital I/O ports (C1 - blue, C2 - yellow and C3 - green) available on the CS110 Power cable (CS110CBL3-L) can be used for a serial digital interface. Control ports C1, C2 and C3 can also be used to conditionally control warning and alarm indicators.

A network or array of electric field meters improves lightning warning because of a wider area of coverage along with measurement redundancy. The PackBus™ communication protocol capability of the CR1000 datalogger embedded in the CS110 provides for extensive networking capability.

7. CRBasic Programming

The CR1000 uses a programming language that has similarities to structured BASIC, hence the name CRBasic. Within CRBasic there are special instructions for making various measurements and for defining tables of output data. Measured results are assigned variable names. Mathematical operations are written out much as they would be algebraically. Conditional statements based on measured results provide users with extensive capability for measurement and control applications. See Section 8 for details on individual instructions. Appendix F contains some example CRBasic programs for the CS110. A simple example CRBasic program illustrating some of the general concepts follows:

```
'Comments can be inserted in CRBasic utilizing a single quote (').
'Simple CS110 program that measures panel (case) temperature, internal case
'relative humidity, battery voltage and electric field.(CS110_Simple.cr1).
'Updated last by Jody Swenson on 7/12/04.

const Mult = 85                                'Define constant to be used in the program.

Public panel_temp                              'Define variables to be used in the program.
Public internal_RH
Public battery_volt
Public E_field
Public leakage_cur
Public status

DataTable(Tab1,1,500)                          'User defined table called Tab1 of size 500 records.
  DataInterval(0,60,sec,10)                    'Output data to the table processed every 60 seconds.
  Average (1,panel_temp,ieee4,0)               'Average panel temperature over interval.
  Average (1,internal_RH,ieee4,0)              'Average internal case RH.
  Average (1,battery_volt,ieee4,0)             'Use 4 byte ieee4 format for wide dynamic range.
  Average(1,E_field,ieee4,0)
  StdDev (1,E_field,ieee4,0)
  Average (1,leakage_cur,ieee4,0)
  Maximum (1,status,ieee4,0,False)
EndTable

BeginProg

  Scan(1,sec,0,0)                              'Scan loop occurring every second.
    PanelTemp (panel_temp,250)                 'Measure temperature on CS110 panel board.
    VoltDiff (internal_RH,1,mV2500,5,True ,0,250,0.1,0)
    Battery (battery_volt)                     'Measure CS110 battery voltage.
    CS110(E_field,leakage_cur,status,_60Hz,Mult,0) 'CS110 electric field measurement.
    CallTable Tab1                             'Call data table Tab1 every scan.
  NextScan
EndProg
```

Public variables are defined and available for viewing in the **Public** table, which is a data table automatically set up by the CR1000. The **Public** table keeps only the current value of each of the defined variables.

In the example program, the **DataTable** instruction is used to define the data table **Tab1**. A record in a table consists of the data from all output processing instructions, along with a record number and time stamp data. Using -1 for last parameter in **DataTable** results in the automatic allocation of all available table storage area. The **DataInterval** instruction following the **DataTable** instruction defines the interval at which new values are determined and written into the table, which is every 60 seconds in the above example. Once a table is full the CR1000 writes new values over the top of old values starting with the oldest data in the table. Data can be collected manually or automatically on a scheduled collection interval by means of LoggerNet PC software.

The **Sample** output processing instruction simply outputs the current variable value at the appropriate time to the data table. The **Average** and **StdDev** output processing instructions accumulate all measured values over the associated data interval and then compute the average and standard deviation, respectively, at the appropriate time. Several other processing instructions exist for the CR1000 as described in the CR1000 Measurement and Control System Operator's Manual.

The **Scan** and **NextScan** instructions set up a loop based on the scan interval. **PanelTemp**, **VoltDiff**, **Battery**, and **CS110** are measurement instructions that return the temperature inside the CS110 case, relative humidity inside the CS110 case, the voltage being provided to the CS110 to power the instrument and the measured electric field, respectively. These and other measurement instructions are discussed more fully in Section 7 on CS110 Measurement Instructions. The **CallTable** instruction sends data to the output processing instructions associated with a given table.

A more involved program that incorporates site correction multiplier, rainfall, wind speed and direction, solar radiation, relative humidity and air temperature, along with electric field follows:

```
'CS110 efield and weather station program.(CS110_WStation.cr1).
'Measures rainfall, wind speed and direction, solar radiation,
'relative humidity and air temperature and electric field.
'Updated last by Jody Swenson on 11/15/05 for Error_Count.

const Mparallel_plate = 85
const Csite = 0.10
const Mcorrected = Mparallel_plate*Csite      'Mcorrected is what goes into CS110 instruction.

Public E_field
Units E_field=volts/m
Public battery_volt
Public leakage_cur
Units leakage_cur=nA
Public status
Public panel_temp
Units panel_temp=DegC
Public rain_fall
Units rain_fall=inch
Public wind_speed
```

```

Units wind_speed=mph
Public wind_dir
Units wind_dir=deg
Public solar_rad
Units solar_rad=W/m2
Public air_temp
Units air_temp=DegF
Public RH
Units RH=%
Public internal_RH
Units internal_RH=%

Public E_status(16)           'E_field status array.
Public k                     'Index for E_status array.
Public meas_error            'Disable variable for slow table.
Public Error_Count          'Keep track of total errors measurements.

DataTable(Tabslow,1,-1)      '-1 to auto-allocate all available memory.
  DataInterval(0,60,sec,10)  'Averaged 60 second output data.
  Average(1,E_field,iieee4,meas_error)
  Sample (1,status,FP2)      'Use 2-byte floating point for non-critical numbers.
  Sample (1,Error_Count,FP2)
  Totalize (16,E_status,FP2,0) 'Look at Efield status array over interval.
  Average (1,leakage_cur,FP2,0)
  Average(1,panel_temp,FP2,0)
  Totalize (1,rain_fall,FP2,0)
  WindVector (1,wind_speed,wind_dir,FP2,False,0,0,0)
  Average (1,solar_rad,FP2,0)
  Average(1,air_temp,FP2,0)
  Average (1,RH,FP2,0)
  Average (1,battery_volt,FP2,0)
  Average (1,internal_RH,FP2,0)
EndTable

DataTable(Tabfast,1,-1)     '-1 to auto-allocate all available memory.
  Sample(1,E_field,iieee4)
  Sample (1,status,FP2)
  Sample (1,leakage_cur,FP2)
  Sample (1,rain_fall,FP2)
  Sample (1,wind_speed,FP2)
  Sample (1,wind_dir,FP2)
  Sample (1,solar_rad,FP2)
  Sample (1,air_temp,FP2)
  Sample (1,RH,FP2)
  Sample (1,battery_volt,FP2)
EndTable

BeginProg

  Error_Count = Tabslow.Error_Count(1,1) 'Retrieve ErrorCount from Tab60sec in case of watchdog.
  if (Error_Count = NAN) Then
    Error_Count = 0
  EndIf

```

```

Scan(1,sec,0,0)
  for k = 1 to 16                                'Initialize status array.
    E_status(k) = 0
  next
  PanelTemp (panel_temp,250)
  Battery (battery_volt)
  VoltDiff (internal_RH,1,mV2500,5,True,0,250,0.1,0)
  PulseCount (rain_fall,1,2,2,0,0.01,0)        'TE525 tipping bucket 0.01 inches per tip
  PulseCount (wind_speed,1,1,1,1,0.2192,0)    'Mult for 05103 Wind Monitor.
  BrHalf (wind_dir,1,mV2500,4,Vx2,1,2500,False,450,250,355,0) 'Mult. for 05103 Wind Monitor.
  VoltDiff (solar_rad,1,mV7_5,3,True,450,250,200,0)
  meas_error = 0                                'Initialize disable variable for Efield average in slow table.
  SW12 (1)                                     'Apply 12 V to warm-up Temp and RH probe at least 150 ms.
  CS110(E_field,leakage_cur,status,_60Hz,Mcorrected,0)
  VoltSe (RH,1,mV2500,1,1,0,250,0.1,0)
  VoltSe (air_temp,1,mV2500,2,1,0,250,.18,-40)
  SW12 (0)                                     'Turn off power to Temp and RH probe.
  if RH > 100 and RH < 108 then
    RH = 100
  EndIf
  If E_field = NAN Then                        'Not-A-Number because of measurement problem.
    meas_error = 1                            'Disable output to slow table if efield = NAN.
  EndIf
  E_status(status) = 1                        'Set appropriate element in status array.
  If status > 6 Then
    Error_Count = Error_Count + 1            'Increment Error_Count.
  EndIf
  CallTable Tabfast
  CallTable Tabslow
  NextScan
EndProg

```

This program incorporates two different user-defined data tables, **Tabfast** and **Tabslow**. **Tabfast** contains 1 second measurements, while **Tabslow** contains 1 minute averaged data. Under certain error conditions the CS110 returns NAN (Not-A-Number) for measured electric field rather than a questionable electric field measurement. For example, the CS110 will detect if the shutter cannot be properly closed at the completion of a measurement due to an obstruction. If the shutter cannot properly close then the CS110 will return NAN for the electric field measurement along with a status value indicating that the motor could not properly close the shutter. The various CS110 status codes are described in Appendix A.

The above program utilizes the array E_status(16) to store the various status codes returned from a given measurement. The **Totalize** instruction in **Tabslow** computes the total number of occurrences for each array value during the output interval. Consequently, the array E_status returns the total number of occurrences of each status code during the associated 1 minute output interval. As given in Appendix A, status codes 1, 2, and 3 are associated with good electric field measurements, whereas each of the higher codes indicates a concerning condition such as low-battery voltage or too much leakage current on the electrode insulators.

There are times when it is desirable to exclude a measured result from an output processing instruction such as **Average**. This can be conveniently

accomplished using a disable variable (**DisableVar**) associated with appropriate output processing instructions. The last parameter of the **Average** instruction is the **DisableVar** and will exclude the current measured value when **DisableVar** is not equal to zero. In order to prevent a single NAN electric field result from corrupting measurements over the entire output interval, the variable `meas_error` is used to disable writing NAN results to the **Average**(1,E_field,iieee4,meas_error) instruction in **TabSlow**.

It is also sometimes desirable to keep a count of total measurement errors, which is accomplished in the above program by the variable `Error_Count`. The last stored value of `Error_Count` is retrieved from final storage at the beginning of the program and `Error_Count` is incremented once during a scan each time status >6 from the **CS110** instruction. The `Error_Count` can be zeroed by means of LoggerNet by accessing the Public variable `Error_Count` in the Numeric display available in the Connect Screen.

Appendix F contains more example CS110 programs that users may find beneficial in various applications. A more detailed description of CRBasic is contained in the CR1000 Measurement and Control System Operator's Manual.

8. CS110 Measurement Instructions

8.1 CR1000 Measurement Overview

The CR1000 datalogger can perform many different measurement tasks as defined by measurement instructions in CRBasic. A brief explanation of CS110 measurement instructions is given followed by some specific examples. Further measurement instructions and measurement details are provided in the CR1000 Measurement and Control System Operator's Manual.

The CR1000 differential voltage measurement (**VoltDiff**) instruction is given as follows:

VoltDiff(Dest,Reps,Range,DiffChan,RevDiff,Settling Time,Integ,Mult,Offset)

where **Dest** is the destination variable of the result. **Reps** is the number of times to repeat a given measurement on successive channels, **Range** is one of ± 5000 mV, ± 2500 mV, ± 250 mV, ± 25 m, ± 7.5 mV, or ± 2.5 mV input voltage ranges available on the CR1000. **DiffChan** is the appropriate differential input channel (1 – 8). **RevDiff** is a true or false parameter to determine whether or not to perform two successive differential measurements with reversed input polarity, in order to reduce low-frequency measurement errors. **Settling Time** is a parameter allowing extra input settling time for “slow” settling sensors. **Integ** is a parameter indicating the length of time to perform an analog integration during the measurement, with options of $250 \mu\text{s}$, $_50\text{Hz}$ and $_60\text{Hz}$. Integration times for $_50\text{Hz}$ and $_60\text{Hz}$ are 20 ms and 16.67 ms, respectively for cancellation of unwanted 50 Hz and 60 Hz noise. **Mult** provides for scaling within the measurement instruction, while **Offset** provides for the incorporation of offsets.

Single-ended voltage measurements are referenced to ground, rather than the low side of a differential input. The **VoltSE** single-ended measurement instruction is quite similar to the **VoltDiff** instruction and is given as follows:

VoltSe (Dest,Reps,Range,SEChan,MeasOff,Settling Time,Integ,Mult,Offset)

An internal ground reference is utilized in single-ended measurements. Single-ended offset errors are reduced in single-ended measurements by measuring the voltage on the internal ground reference. The **MeasOff** parameter in the **VoltSe** instruction determines if this internal ground reference is measured at the beginning of every **VoltSe** instruction (**MeasOff** = True) or whether a single-ended offset voltage measure is performed as part of an on-going instrument self-calibration routine occurring in background (**MeasOff** = False).

Another general purpose voltage measurement instruction is the **BrHalf** instruction, which provides voltage excitation for a simple resistive divider (half of a 4-element Wheatstone bridge), and then measures the resulting voltage.

A **BrHalf** instruction follows:

BrHalf (Dest,Reps,Range,SEChan,ExChan,MeasPEX,ExmV,RevEx,Settling Time,Integ,Mult,Offset)

Most parameters of the **BrHalf** instruction are common to the **VoltDiff** and **VoltSE** instructions, and so only the differences will be discussed. The **ExChan** parameter determines which one of the three CR1000 voltage excitation outputs are used to excite the half-bridge. **MeasPEX** determines how many successive channels are excited by the same excitation channel in successive **Reps**. **ExmV** determines the excitation voltage which can range from -2500 mV to +2500 mV. **RevEx** is a true/false parameter and if true then the polarity of the excitation is reversed during the measurement and a second measurement taken. Like input reversal on differential measurements, excitation reversal is an error canceling technique for reducing low-frequency measurement errors such as offset voltages.

The **Battery** instruction is used to measure the input voltage of the power supply to the CS110 and follows:

Battery (Dest)

The **PanelTemp** instruction is used to measure the temperature of a thermistor located within the CS110 case and follows:

PanelTemp (Dest,Integ)

The **PulseCount** instruction is used to count the pulses generated from sensors, such as an anemometer or switch closures from a tipping bucket rain gauge, and has the following parameters.

PulseCount(Dest,Reps,PChan,PConfig,POption,Mult,Offset)

PChan is the number pulse channel (1 or 2) used for the measurement. **PConfig** is a code (0-2) for three different types of pulse-count inputs; High-frequency = 0, low-level AC = 1, and switch closure = 2. **POption** is a code to

determine if results are returned as counts for a given interval (**POption** = 0), or as frequency = counts/(scan interval in seconds) (**POption** = 1).

8.2 Measuring Electric Field

The **CS110** instruction is used to perform the electric field measurement of the CS110 and follows:

CS110(Dest,Leakage,Status,Integ,Mult,Offset)

Leakage is a variable containing the measured leakage current in nano amps (nA) on the charge amplifier input during the CS110 electric field measurement. A perfect unit is 0 nA. Actual units deviate from perfection such that some have small ($\ll 1$ nA) positive leakage current and some have small negative leakage current. **Status** is a variable containing numeric codes indicating various status conditions occurring during the measurement, as defined in Appendix A. **Integ** is a parameter indicating the length of time to perform an analog integration during the measurement, with options of 250 μ s, **_50Hz** and **_60Hz**. Integration times for **_50Hz** and **_60Hz** are 20 ms and 16.67 ms, respectively for cancellation of unwanted 50 Hz and 60 Hz noise. **Mult** provides for convenient scaling within the measurement instruction, and **Offset** provides for convenient incorporation of offsets. The CS110 instruction measures the electric field utilizing the ± 250 mV range. If the result is NAN, the instruction re-measures utilizing the ± 2500 mV input voltage range.

8.3 Measuring Electric Field Change

CS110Shutter(Status,Move)

Status is a variable containing the following subset of measurement status codes given in Appendix A: status codes 1, 4, 7, 8, 9, 10, 11, 14, 15, and 16.

Move is a variable set to 1 to open the shutter and set to 0 for the **CS110Shutter** instruction to close the shutter.

The **CS110Shutter** instruction can be utilized along with a **Delay** instruction to visually verify the fully opened and fully closed positioning of the CS110 shutter, as described in Appendix D on Servicing the CS110. The **CS110Shutter** instruction can also be used to implement a Slow Antenna electric field measurement as described in Appendix E. The CS110 panel board contains circuitry to switch in a parallel 200 M Ω resistor with the 330 pf feedback capacitor in the charge amplifier during execution of an open shutter **CS110Shutter** instruction. This results in a charge amplifier with a 66 ms time constant implemented as a slow antenna that can be utilized to measure changes in electric field at rates much faster than the 5 Hz maximum rate of the **CS110** electric field measurement instruction. In the slow antenna mode the CS110 becomes a field-change meter, meaning that the useful data becomes the differences between the **VoltDiff** measurements rather than the absolute value of each **VoltDiff** measurement.

8.4 Measuring Solar Radiation or Barometric Pressure

Circular connector labeled **SOLAR RADIATION** on the CS110 can be used to connect up an LI200X solar radiation sensor. Alternately, a special cable, the CS110-L BAROMETRIC PRESSURE SENSOR CABLE (17460), can be

purchased and connected to the **SOLAR RADIATION** connector to interface to either the CS100 or the CS106 barometric pressure sensor. Examples of instructions to measure the LI200X solar radiation sensor or the barometric pressure sensors are given below.

```

'Measure LI200X.
  VoltDiff (solar_rad,1,mV7_5,3,True,450,250,200,0)

'Measure CS106 - "continuous" or "always on" mode = jumper installed
  VoltDiff (Barom_pres,1,mV2500,3,True,450,250,0.24,500)

'Measure CS100 every hour - "triggered" mode = on/off. Trigger or turn on by setting control port
4 (C4=green wire) high.

  Scan (1,Sec,0,0)

  If Iftime(3599,3600,sec) then PortSet (4,1 )

  VoltDiff (Barom_pres,1,mV2500,3,True,450,250,0.2,600)

  If Iftime(0,3600,sec) then PortSet (4,0 )

  NextScan
    
```

8.5 Measuring Air Temperature and Relative Humidity

Circular connector labeled **TEMP/RH** can be used to connect up an HC2S3 temperature and relative humidity sensor. Example CRBasic instructions to measure the HC2S3 Temperature and RH are given below.

```

SW12 (1 )           'Apply switched 12 V power to the probe.
Delay (0,3,sec)     'Warm up probe before measurements.
VoltSe (air_temp,1,mV2500,2,1,0,250,-18,-40) 'Single-ended air temp. measure.
VoltSe (RH,1,mV2500,1,1,0,250,0.1,0)       'Single-ended relative humidity.
SW12 (0)           'Turn off power to the probe.
if RH > 100 and RH < 103 then
RH = 100
Endif
    
```

8.6 Measuring Wind Speed and Direction

Circular connector labeled **WIND** can be used to connect up various wind sensors, including the 05103 Wind Monitor, 034B Met One Wind Sensor, and 03001 Wind Sentry. Example CRBasic instructions to measure the 05103 Wind Monitor are given below.

```

PulseCount (wind_speed,1,1,1,1,0.2192,0)      'Wind Speed.
BrHalf (wind_dir,1,mV2500,4,Vx2,1,2500,False,450,250,355,0) 'Wind Direction.
    
```

8.7 Measuring Rainfall

Circular connector labeled **RAIN** can be used to connect up a rain gauge using a switch closure such as the CS700 or the TE525MM tipping bucket rain gauges. Example CRBasic instruction to measure the TE525 is given below.

PulseCount(rain_fall,1,2,2,0,0.01,0)	<i>TE525 tipping bucket 0.01 inches per tip</i>
--------------------------------------	---

8.8 Measuring Internal Case Humidity

In order to determine when to change desiccant within a CS110 case, a relative humidity sensor is contained inside the case. The following CRBasic instruction provides internal humidity data to the variable Internal_RH, which can then be monitored in real-time and/or included in an output table.

VoltDiff(Internal_RH,1,mV2500,5,True,0,250,0.1,0) 'Internal humidity measure.

Changing of CS110 desiccant is recommended for internal relative humidity values $\geq 80\%$.

9. PC Software

Campbell Scientific offers two datalogger support software packages for PC computers that can be used with the CS110 and its embedded CR1000 datalogger. The PC400 package is less expensive than the full featured LoggerNet package but PC400 does not support combined communication options (e.g., phone-to-RF), PakBus routing, or scheduled data collection. LoggerNet software is recommended for applications that require these capabilities.

The CS110's embedded CR1000 datalogger is only supported in LoggerNet version 3.0 and higher or PC400 version 1.0 and higher. Upgrades to earlier versions of LoggerNet or PC208W are available for approximately half the list price.

The following overview describes connecting a PC running LoggerNet to the CS110 and viewing electric field data. The full capabilities of LoggerNet and PC400 are covered in their respective manuals.



9.1 Quick Start


Connect the CS110's RS232 port to the PC, and apply 12 Vdc power to the CS110. Due to a factory installed CR1000 program the shutter should begin to open/close about 30 seconds after power is turned on.

The CR1000 uses a Campbell Scientific communication protocol called PakBus. Each CR1000 datalogger in a network connecting to the LoggerNet PC should have a unique PakBus address. Each CS110 is shipped with a PakBus address of 1.

The following three screen captures show the settings for each of the three links in the path from COM Port 1 on the PC to the CS110 with the factory


default PakBus address of 1. Use LoggerNet Tool Bar's "Setup" button or "EZ Setup" button to create the PC to CS110 communication path shown below:

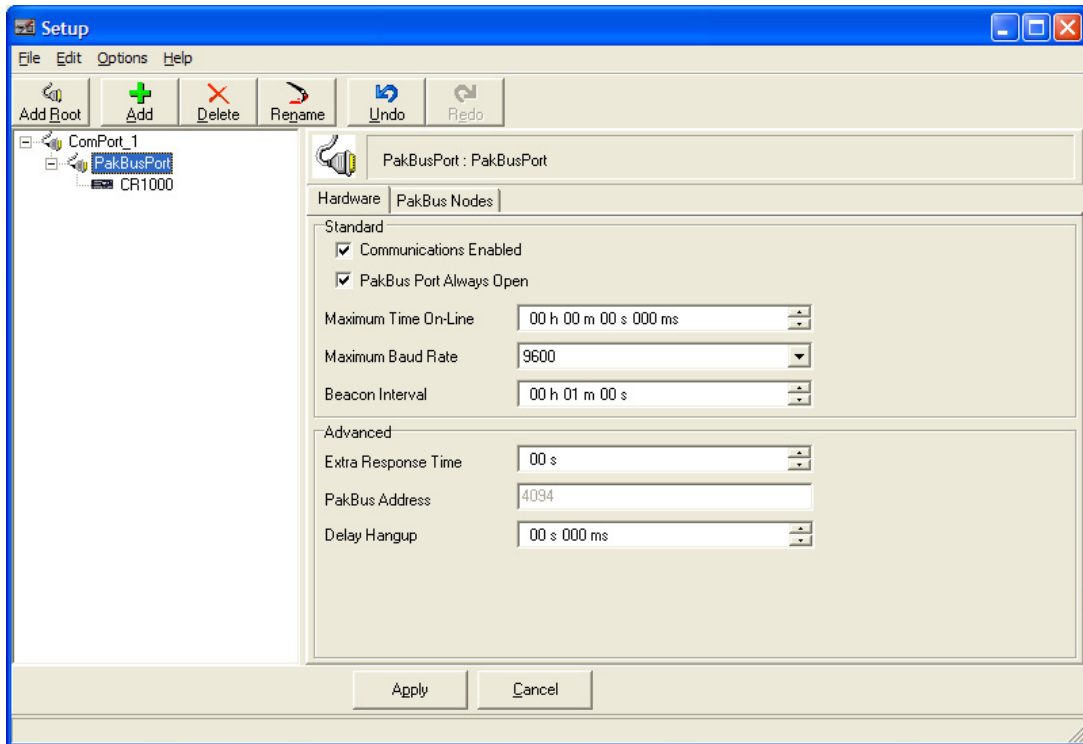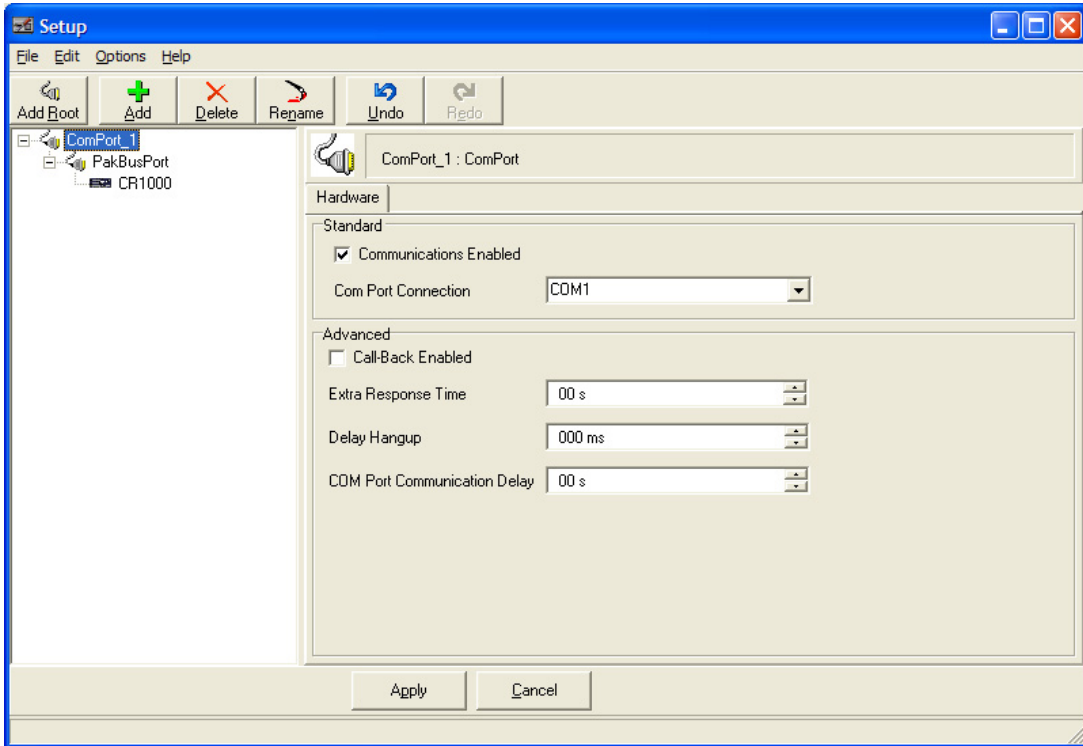

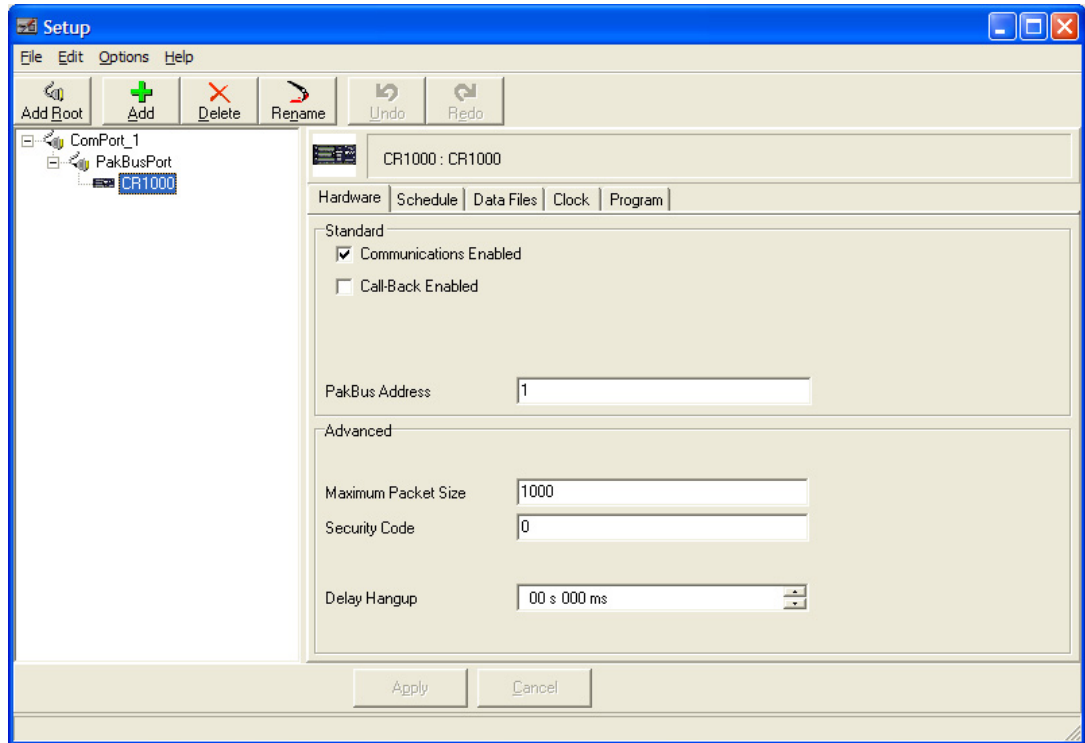

Remember to click on the “Apply” button to cause the settings to take effect. The “Apply” button is grayed out once it has been executed.

Once this is done, switch to the “Connect” button on the LoggerNet Tool Bar, select the CS110, and select “Connect”.

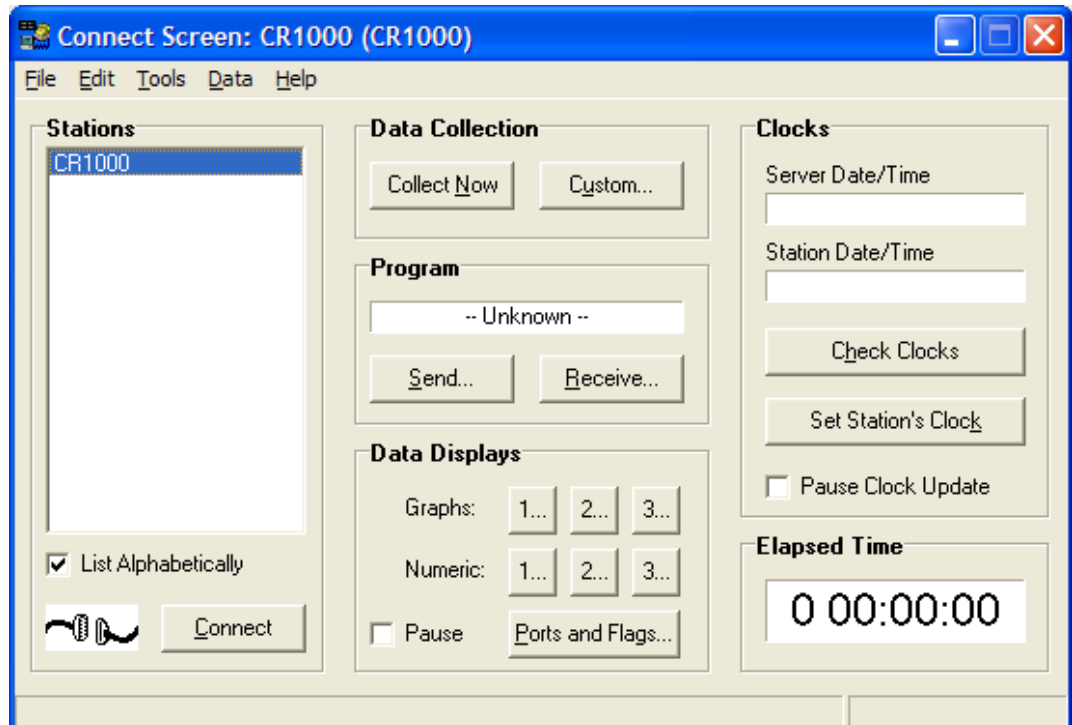



If the connection is made and the stations time shows up in the window, you can then select the “Numeric:” button and add the desired public variables to see electric field readings updated every measurement interval.

If you have changed the CR1000’s PakBus address and subsequently forgotten it, you can download from <http://www.campbellsci.com/downloads> at no cost, a software package named Device Configuration Utility that will discover the PakBus address. Run the software and set it up with device type set to CR1000, specify the correct COM port, and select “Connect” and the software will discover the PakBus address for you.

If necessary, this software is also used to send a new operating system (OS) to the CR1000.

The following screen captures show the Device Configuration software.

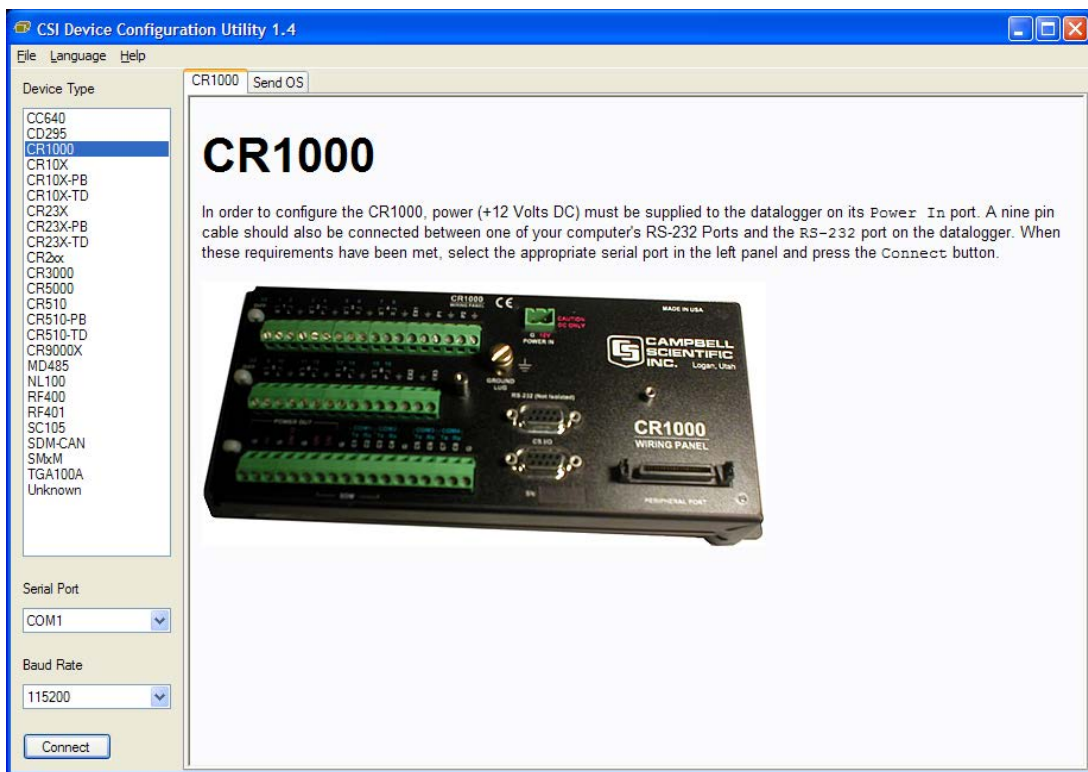

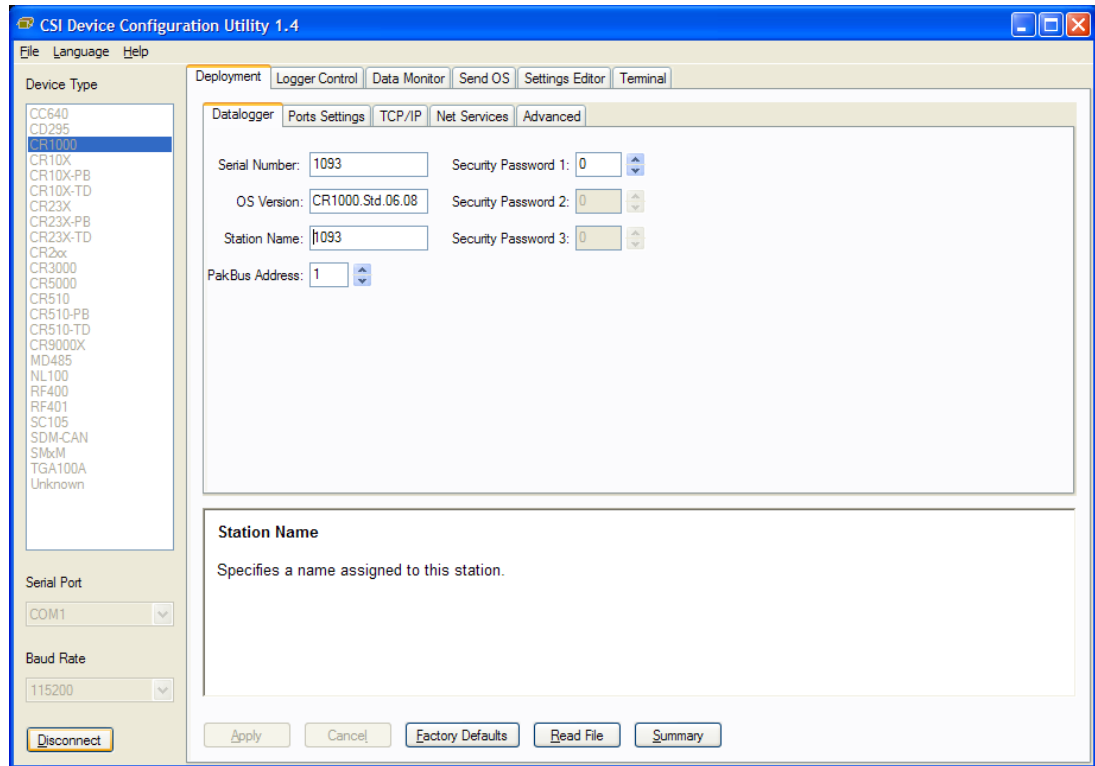

10. Maintenance

10.1 Checking Site Ground Integrity

The CS110 electric field meter needs to be electrically connected to Earth ground for valid measurements. It is recommended that the integrity of this Earth Ground connection be checked periodically by verifying that the resistance of the stator to Earth Ground rod is $<1 \Omega$.

10.2 Corrosion and Rust Inhibitors

In corrosive environments, metal friction points (set screws, bolts, etc.) and electrical connections to earth ground can be protected with the use of a rust inhibitor. Sanchem makes such an inhibitor and some information on their products may be found at <http://www.sanchem.com/ox.html>. Following is an excerpt from their web site:

“NO-OX-ID A-SPECIAL is a soft, wax based rust preventive and lubricant that contains an active rust inhibitor and small amount of solvent for ease of application. This corrosion resistant coating can be applied by spray or brush application. NO-OX-ID A-SPECIAL controls corrosion by leaving a thick, semi-transparent, non-drying barrier coating that retains its anti-rust properties indefinitely.

NO-OX-ID A-SPECIAL is the electrical contact grease of choice in new electrical installations and maintenance because of its excellent performance in keeping metals free from corrosion. This rust preventative has been used for over 50 years to prevent corrosion in electrical connectors from low micro-

power electronics to high voltage switchgear. NO-OX-ID A-SPECIAL prevents the formation of oxides, sulfides and other corrosion deposits on copper surfaces and conductors can be prevented with its use.”

Loctite also makes a similar product and some information on their products may be found at <http://content.loctite.com/sticks/silver-as.html>. Following is an excerpt from their web site:



Heavy-duty, temperature-resistant up to 1600°F, petroleum-based lubricant fortified with graphite and metallic flake.

Features and Benefits

- Protects metal parts in high heat environments up to 1600°F
- Prevents rust, corrosion, seizing and eases disassembly
- Reduces friction and wear to critical parts
- Buttery texture ideal for both coarse and fine threads
- Exceptional lubrication properties

Typical Applications

- For use with copper, brass, cast iron and all alloys including stainless steel, all plastics and all non-metallic gasket materials
- Bolts, bushings, pipes, fittings, flanges, gaskets, headers, manifolds, nuts, studs, etc.
- High heat ovens
- Crane assemblies

- Turbine studs
- Coal crushers
- Casting and Molding equipment
- Heat exchangers

10.3 Self-Check Features

The CS110 has been designed to provide reliable electric field measurements and to simplify and minimize maintenance. Scheduled maintenance may not be required, as the CS110 incorporates extensive self-checking, and provides status information about each measurement. An example CS110 instruction follows.

CS110(E_field,leakage_cur,status,_60Hz,Mult,Offset)

Returned **E_field** values of NAN (Not-A-Number) indicate a measurement problem that can be determined from the associated **status** value.

The **status** parameter returned from each electric field measurement reports of measurement problems along with instrument health. The CS110 **status** values are described in Appendix A.

The **leakage** parameter returns the measured charge amplifier input leakage current. A perfect unit is 0 nA. Actual units deviate from perfection such that some have small ($\ll 1$ nA) positive leakage current and some have small negative leakage current. Occasional leakage current values exceeding ± 4.2 nA may occur if insulators are wet. If leakage current values return to < 1.0 nA upon drying then no service is required. However, prolonged leakage current values near to and exceeding 4.2 nA are likely due to insulator contamination requiring removal of the stator and cleaning.

10.4 Cleaning the CS110 Electrode Head

The CS110 motor assembly illustrating the 316-L stainless-steel stator, shutter, and sense electrode is illustrated in Figure 13.

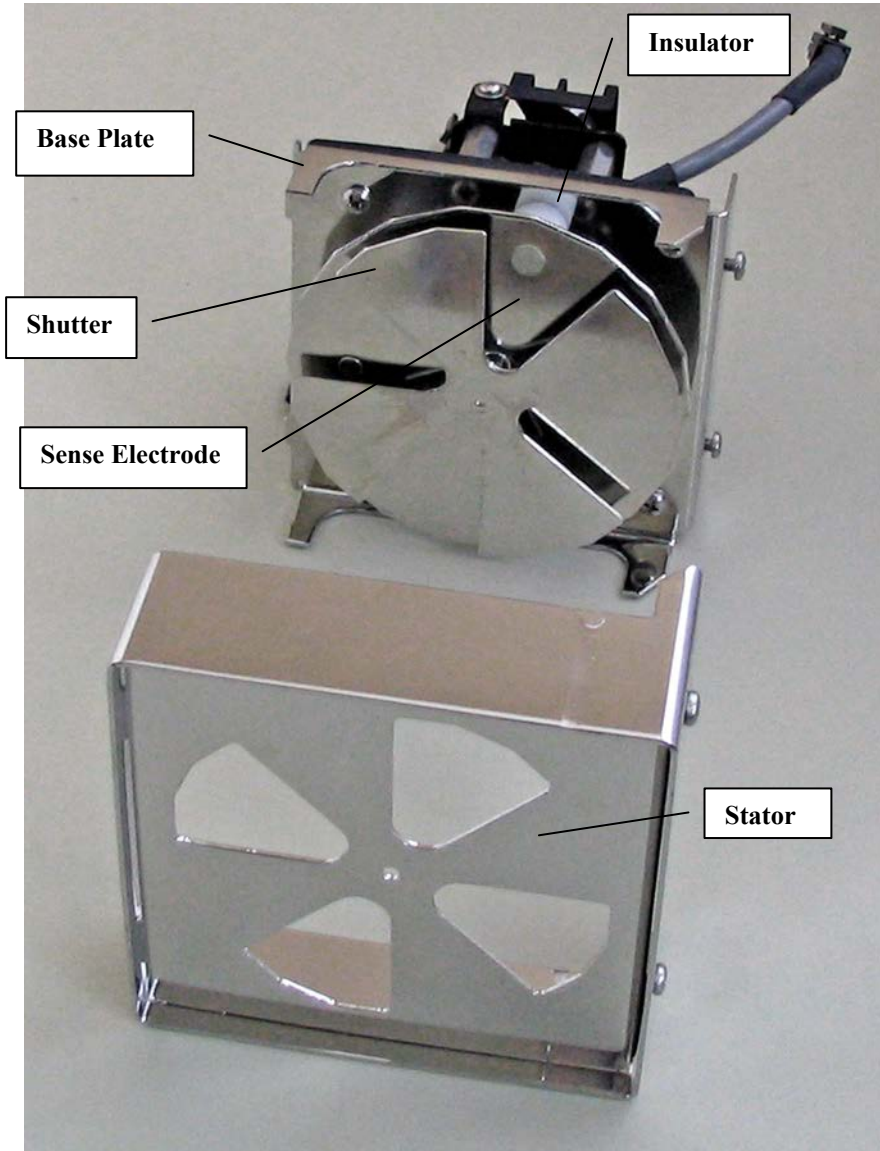


FIGURE 13. CS110 stator, shutter and sense electrode

Contamination of the polished stator, shutter, and sense electrode can result in unwanted surface charges that induce electric field offset errors in the measurement.

Three Teflon insulators are utilized to electrically insulate the high-impedance sense electrode from the motor assembly base plate. Surface contamination of these insulators can result in excessive leakage current. The CS110 includes a circuit to compensate for input leakage current on the charge amplifier up to

± 4.2 nA. Leakage current values in excess of ± 4.2 nA can cause measurement errors and are indicated by **status** = 11.

Cleaning of the CS110 electrodes and/or insulators is recommended if any of the following conditions occur:

- When insulators are dry, and leakage current exceeds ± 4.2 nA as indicated by **status** = 11.
- Visual evidence of contamination (salt deposits, scaling, dust, spider webs etc.) on or around electrode area.
- Zero field reading with Zero Electric Field Cover (PN: 17642) exceeds ± 60 V/m. Note: it is important that the inside of the zero field cover also be clean for good zero field reading.

Electrode Cleaning Procedure:

1. Remove the stator by loosening the 2 Philips head screws on the motor assembly base plate, allowing the stator to pivot and be removed.
2. Inspect the stator for any contaminant deposits and scrub such deposits off with soap and hot water if available. Any residue may form non-conductive layers that can hold unwanted surface charge. Using a brush that will fit between the shutter and the sense electrode, carefully wash the shutter and sense electrode, along with the three insulators attaching the sense electrode to the main body of the CS110. One brush (CSI PN 17578) ships with each CS110. Large offsets are likely due to electrical charges residing insulative deposits on metallic surfaces, while large leakage currents are likely due to contaminated insulators.
3. Rinse well, using de-ionized water if available, and blow dry with air.
Note: Rubbing and wiping tends to induce unwanted surface charging that will eventually dissipate.
4. Reassemble the stator making sure it is positioned properly before tightening the two Philips head stator screws. Try and avoid getting fingerprints, etc. on clean electrodes as they can result in unwanted surface charge. (Clean cotton gloves are helpful.)
5. Attach the zero field cover plate (PN: 17642) to the stator and verify that the leakage current $\leq |0.5 \text{ nA}|$ and that the zero field offset $\leq 60 \text{ V/m}$. Leakage current $> |0.5 \text{ nA}|$ and/or zero field offsets $> 60 \text{ V/m}$ indicate problems with cleanliness and/or unwanted surface charge.

10.5 Changing Desiccant

The CS110 is shipped with desiccant inside the sealed case to reduce humidity for the sensitive electronics enclosed. A humidity sensor is also contained inside the CS110 case to allow monitoring of the internal relative humidity. The following CRBasic instruction provides internal humidity data to the variable **Internal_RH**, which can be included in an output table.

VoltDiff(Internal_RH,1,mV2500,5,True,0,250,0.1,0) 'Internal humidity measure.

Changing of CS110 desiccant is recommended for internal relative humidity values $\geq 80\%$.



FIGURE 14. Inside of CS110 case illustrating bracket for holding desiccant

NOTE

Replacement intervals less than once every six months for the 4 Unit (PN: 4905) desiccant pack within the sealed CS110 case indicate a problem with the CS110 case seal or with the desiccant packs being used.

Procedure for Changing Desiccant:

1. Remove the CS110 case lid by unscrewing the captive screws that attach the lid to the main body of the CS110.

2. Inspect the gasket on the CS110 lid making sure that a good seal is possible when the lid is replaced.
3. Remove the old desiccant pack and replace with a new 4 unit desiccant pack (PN: 4905) making sure the new pack is placed into the bracket that prevents the desiccant from sliding into the motor assembly.

10.6 Checking Shutter/Encoder Alignment

Status codes 14, 15, and 16 indicate problems with the stepper motor correctly opening and closing the shutter. A mechanical trim procedure is done at the factory to set proper shutter/encoder alignment, as described in Appendix D. Proper shutter/encoder alignment can be verified with the following procedure utilizing the special **CS110Shutter** instruction which positions the shutter in the fully closed or fully open positions. The following program combines the **CS110Shutter** instruction with **Delay** instructions so that fully closed and fully open shutter positions can be verified visually. Stator to shutter overlap exists in the fully opened and fully closed positions so that slight shutter position variations do not alter the exposed area to the sense electrode. A fully opened shutter will display symmetrical stator to shutter overlap, within the 1.8° stepper motor step size, on both edges of each of the 4 openings in the stator when viewed from a perpendicular position to the direction of the shutter blades. No visible gaps between the stator and shutter blades should be visible on a fully closed shutter when viewed from a position perpendicular to the shutter blades.

*'Program to open/close the CS110 shutter (CS110_Shutter1.cr1).
'Last updated by Jody Swenson on 9/26/05.*

```
Public PTemp
Public Batt
Public stat(2)
```

```
DataTable(Efield,1,-1)
  Sample(2,stat,FP2)
  Sample(1,PTemp,IEEE4)
  Sample(1,Batt,IEEE4)
EndTable
```

```
BeginProg
```

```
  Scan(5000,msec,0,0)
    PanelTemp(PTemp,250)
    Battery(Batt)
    CS110Shutter(stat(1),1)           'Fully open shutter.
    Delay (0,3000,mSec)
    CS110Shutter(stat(2),0)         'Fully close shutter.
    CallTable Efield
```

```
  NextScan
EndProg
```

10.7 Re-Calibration

Re-calibration of measurement instruments is commonly done in data critical applications in order to combat component drift with time. Component drift is a function of the environment experienced by the instrument. High humidity and/or high temperature environments generally cause the most drift. For the CR1000 datalogger a two year re-calibration interval is recommended, with longer intervals being sensible for users that find negligible instrument drift over a two year period. The embedded CR1000 datalogger inside the CS110 case should experience a low-humidity environment, which helps minimize datalogger measurement drift.

As mentioned in Section 5.1, each CS110 is factory calibrated in the parallel plate calibrator illustrated in Figure 5 to determine individual instrument gain. The CS110 electric field measurement instrument gain is a function of electrode dimensions, along with the 1% feedback capacitor used in the charge amplifier. While measurement drift of CR1000 is likely negligible with regard to the $\pm 5\%$ of reading accuracy specification of electric field measurements, datalogger drift may be a factor for the measurement of temperature by means of an external temperature and RH probe.

A parallel-plate calibration is recommended whenever any electrodes are bent, removed or replaced, with the exception of the removal and replacement of the same stator during the process of insulator cleaning. For CS110 applications requiring long-term electric field measurement accuracy better than $\pm 10\%$, a parallel plate factory calibration is recommended every three years.

The expected lifetime of the CS110 is 5 to 10 years, again depending upon the operational environment. Instruments operated in coastal environments will likely suffer from external finish degradation and/or operational failure sooner than instruments operated in dry inland environments.

11. References

“Lightning Physics and Effects” by Vladimir A. Rakov and Martin A. Uman, Cambridge University Press, 2003.

“The Electrical Nature of Storms” by Donald R. MacGorman, and W. David Rust, Oxford University Press, Inc., 1998.

“On some determinations of the sign and magnitude of electric discharges in lightning flashes” by C.T.R. Wilson, *Proceedings of the Royal Society*, Series A, Vol. 92, 555-574, 1916.

“Industrial Electrostatics – fundamentals and measurements” by D.M. Taylor and P.E. Secker, John Wiley & Sons Inc. 1994, pg. 36-38.

(LPLWS) METEOROLOGICAL\CCAFS\81900\LAUNCH PAD
LIGHTNING WARNING SYSTEM
(<http://www-sdd.fsl.noaa.gov/RSA/lplws/LPLWS-handbook.Apr03.pdf>).
Please note that the web site address is case sensitive.

NOAA (See www.lightningsafety.noaa.gov/outdoors.htm.)

NAVSEA OP 5, Vol 1, Seventh Rev. Para 6-2, pg 6-1 and 6-2, 2001.

Appendix A. CS110 Measurement Status Codes

Status codes 1 through 3: Good Instrument Health.

status = 1, Good instrument health. ± 250 mV measurement range only. Return measured Efield value.

status = 2, Good instrument health. ± 2500 mV measurement range used. Return measured Efield value.

status = 3, Good instrument health. NAN returned for Efield because of measurement over-range on the ± 2500 mV measurement range.

No priority issues exist with status codes 1 through 3 since only 1 of these “Good Instrument Health” codes can exist for a given measurement.

Status codes 4 through 6: Good measurement, after properly positioning the shutter.

status = 4, Good instrument health. ± 250 mV measurement range only. Had to properly position shutter.

status = 5, Good instrument health. ± 2500 mV measurement range used. Had to properly position shutter.

status = 6, Good instrument health. NAN returned for Efield because of measurement over-range on the ± 2500 mV measurement range. Had to properly position shutter.

Status code 4 through 6 indicate that the shutter was not properly positioned upon commencing the measurement. The problem was recognized, corrected and a valid measurement made. Status codes 4 through 6 are common upon power up, or if the shutter has been touched or bumped since the last execution of the CS110 instruction. Persisting status codes 4 through 6 indicate a problem with parking the shutter that should be investigated.

Status codes 7 through 10: Datalogger warnings and errors.

status = 7, +5Vext low. Return measured Efield value.

status = 8, Datalogger skipped scan. Return measured Efield value.

status = 9, Input power < 9.6 V. Return measured Efield value.

status = 10, Datalogger watchdog reset. Return measured Efield value.

Status codes 7, through 10 increase in priority with 7 being the lowest and 10 the highest of the warning and error codes. Status code 7 is a low priority error message, as low +5Vext is a concern, but does not corrupt electric field measurements. Status code 7 is overwritten by any other warning and error code (i.e. $\text{status} \geq 7$), including Leakage current exceeds compensation range.

Status codes 8 through 10 are the highest priority error messages returned by the CS110, and will overwrite other lesser errors that occur simultaneously during the CS110 instruction. Since only one status value can be returned from a CS110 instruction, status 10 is given the highest priority, status 9 the second highest, and 8 the third highest priority of CS110 status codes. Next in priority are codes 16, 15, 14, 13, 12, and 11 followed by 7, 6, 5, 4, 3, 2 and 1.

Status codes 11 through 16: Measurement warnings and errors.

status = 11, Leakage current exceeds compensation range of ± 4.2 nA. Return measured Efield value.

status = 12 Failed charge-amplifier self check. Return NAN instead of measured Efield value.

status = 13, Large closed shutter offset voltage. $V_{os} > |1.00 \text{ V}|$. Return NAN instead of measured Efield value.

status = 14, Motor move error. Incorrect number of motor steps to close shutter. Return NAN instead of measured Efield value.

status = 15, Motor move error. Encoder UPCNTs < 24 or > 26 . Encoder DNCNTs < 24 or > 26 , or don't find home when closing. Return NAN instead of measured Efield value.

status = 16, Can't properly position shutter. Return NAN instead of measured Efield value.

Status code 11 returns the measured Efield value because the electric field computation algorithm compensates for leakage current, even if it exceeds ± 4.2 nA, although maximum signal amplitude becomes limited. **Consequently, cleaning of the instrument is recommended if status code 11 persists for long periods of time.**

Status codes 12 through 16 all cause the measured electric field to be set to NAN in order to prevent the use of possible erroneous measurements. The priority of codes 11 through 16 increases with increasing values, although codes 8, 9 and 10 are higher priority.

Appendix B. CS110 Accessories

B.1 Zero Electric Field Cover

As previously mentioned, unwanted surface charges residing on non-conductive deposits on electrodes result in a non-zero electric field, even when external electric fields are zero. Polished 316-L stainless-steel is used for critical electrode surfaces on the CS110 to minimize unwanted surface charges. CS110's with clean electrodes have been found to display electric field offsets less than 20 V/m in absolute value. The CS110 Zero Electric Field Cover (PN: 17642) is used to check the electric field offset voltage of the CS110. If the measured electric field is $\geq |60 \text{ V/m}|$ with the Zero Electric Field Cover on, then inspection and cleaning of the electrode surfaces as discussed in Section 10.4 is recommended.

B.2 Upward-Facing Site Calibration Kit

As previously mentioned, the CS110 is calibrated in a parallel plate calibration chamber, resulting in a valid calibration for a flush-mounted upward-facing configuration. Yet, inverted and elevated CS110 mounting configurations are recommended for long term installations. Upward-facing site calibration kit (PN: 17579) has been designed to provide a flush-mounted upward-facing configuration for the CS110 to aid in determining site correction factors.

B.3 CR1000 Keyboard Display


The CR1000 keyboard display (CR1000KD) is a convenient CR1000 user interface that can be directly connected to the CS110. The CR1000 keyboard display connects to the CS110 through the CS I/O port, requiring a CS110 CS I/O Cable (CS110CBL2-L). The CR1000KD can be used to view data and programs, and to make simple program modifications. Details on the CR1000KD can be found in the CR1000 Measurement and Control System Operators Manual.

B.4 Miscellaneous Peripheral Modules

The CS110 is compatible with CSI SDM (Synchronous Device for Measurement) peripherals. The C1, C2, and C3 control ports necessary for SDM are available through the CS110 POWER CABLE (CS110CBL3-L). SDI-12 sensors can also be read using C1 and/or C3.

Appendix C. CS110 Connector Pin-outs

The following information describes the connectors that mate with the built-in (bulkhead) connectors on the CS110. Connector pin numbering for the 6 and 9 pin connectors are shown below. The view is a view of the solder-cup side of the cabled connector. The circular connectors are Mini-Con-X type from Conxall. The CSI part numbers shown for the connectors include the backshell. CSI fills the backshell with a relatively thick epoxy to seal and provide strain relief.

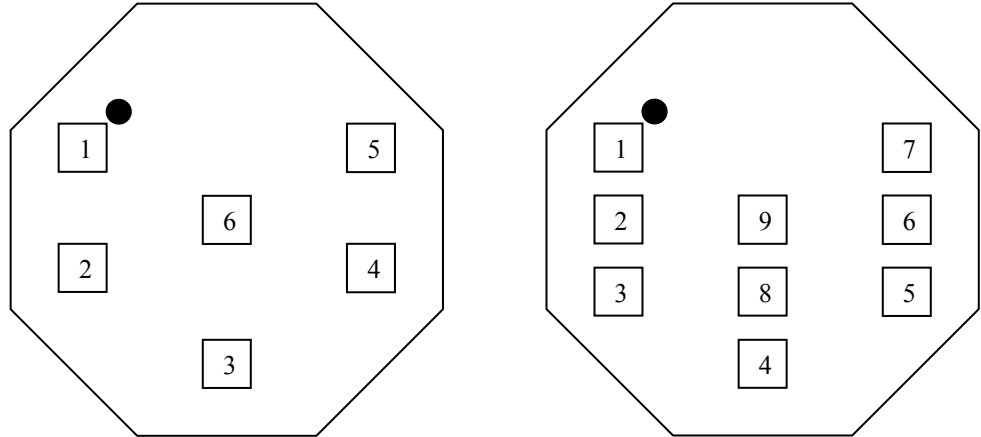

POWER CONNECTOR

CS110CBL3-L CS110 Power Cable

Connector is female and is CSI PN 17654 (Conxall #6282-6SG-522 or Switchcraft #EN3C6F). Pin 1 is indicated with a dot.

Pin	Description	Color
1	C1 Control Port 1	Blue
2	+12 V Power	Red
3	Gnd Digital Ground	Drain (clear)
4	P_Gnd Power Ground	Black
5	C3 Control Port 3	Green
6	C2 Control Port 2	Yellow

WIND CONNECTOR

Connector is male and is CSI PN 9889 (Conxall #6282-6PG-522 or Switchcraft #EN3C6M). Pin 1 is indicated with a dot.

Pin	Description
1	2LO Single-ended channel 4
1	1Mohm Pin 1 also connects to ground via a 1 Mohm 1% 50ppm resistor
2	Gnd Panel Ground
3	EX2 Excitation channel 2
4	P1 Pulse channel 1
5	Gnd Power ground
6	Gnd Ground

RAIN CONNECTOR

Connector is male and is CSI PN 9889 (Conxall #6282-6PG-522 or Switchcraft #EN3C6M). Pin 1 is indicated w/ a dot

Pin	Description	Color
1	empty	
2	empty	
3	P2	Pulse channel 2
4	empty	
5	Gnd	Power ground
6	Gnd	Power ground

CSIO CONNECTOR

CS110CBL2-L CS110 CS I/O Cable

Connector is 9 pin female and is CSI PN 17674 (Conxall #3082-9SG-330). Pin 1 is indicated w/ a dot

Pin	Description	Color
1	+5V	+5 Volt dc supply
2	Gnd	Power ground
3	Ring	Ring
4	RX	Receive
5	ME	Modem enable
6	SDE	Synchronous device enable
7	CLKHS	Clock hand shake
8	+12V	+12 Volt dc supply
9	TX	Transmit

RS-232 CONNECTOR

CS110CBL1-L CS110 RS-232 Cable

Connector is 9 pin male and is CSI PN 15880 (Conxall #3282-9PG-330). Pin 1 is indicated w/ a dot

Pin	Description	Color
1	DTR	Data terminal ready
2	TX	Transmit
3	RX	Receive
4	empty	
5	Gnd	Power ground
6	DTR	Tied to pin 1
7	CTS	Clear to send
8	RTS	Request to send
9	Ring	Ring

SOLAR RADIATION CONNECTOR

Connector is male and is CSI PN 9889 (Conxall #6282-6PG-522 or Switchcraft #EN3C6M). Pin 1 is indicated w/ a dot

<u>Pin</u>	<u>Description</u>	
1	3HI	Single-ended channel 5 or high side of differential channel 3
2	3LO	Single-ended channel 6 or low side of differential channel 3
3	+12V	+12 Volt dc supply
4	C4	Control port 4
5	C3	Control port 3
6	Gnd	Power ground

TEMP/RH CONNECTOR

Connector is male and is CSI PN 9889 (Conxall #6282-6PG-522 or Switchcraft #EN3C6M). Pin 1 is indicated w/ a dot

<u>Pin</u>	<u>Description</u>	<u>Color</u>
1	1HI	Single-ended channel 1 or high side of differential channel 1
2	1LO	Single-ended channel 2 or low side of differential channel 1
2	1Kohm	Pin 2 also connects to ground via a 1 Kohm 0.1% 10 ppm/C resistor
3	empty	
4	+12Vsw	Switched +12 volt dc supply
5	Gnd	Ground
6	Gnd	Power ground

Appendix D. Servicing the CS110

The CS110 has been designed to provide reliable electric field measurements and to simplify and minimize maintenance. An exploded view illustrating the various major components of the CS110 is illustrated in Figure D-1.

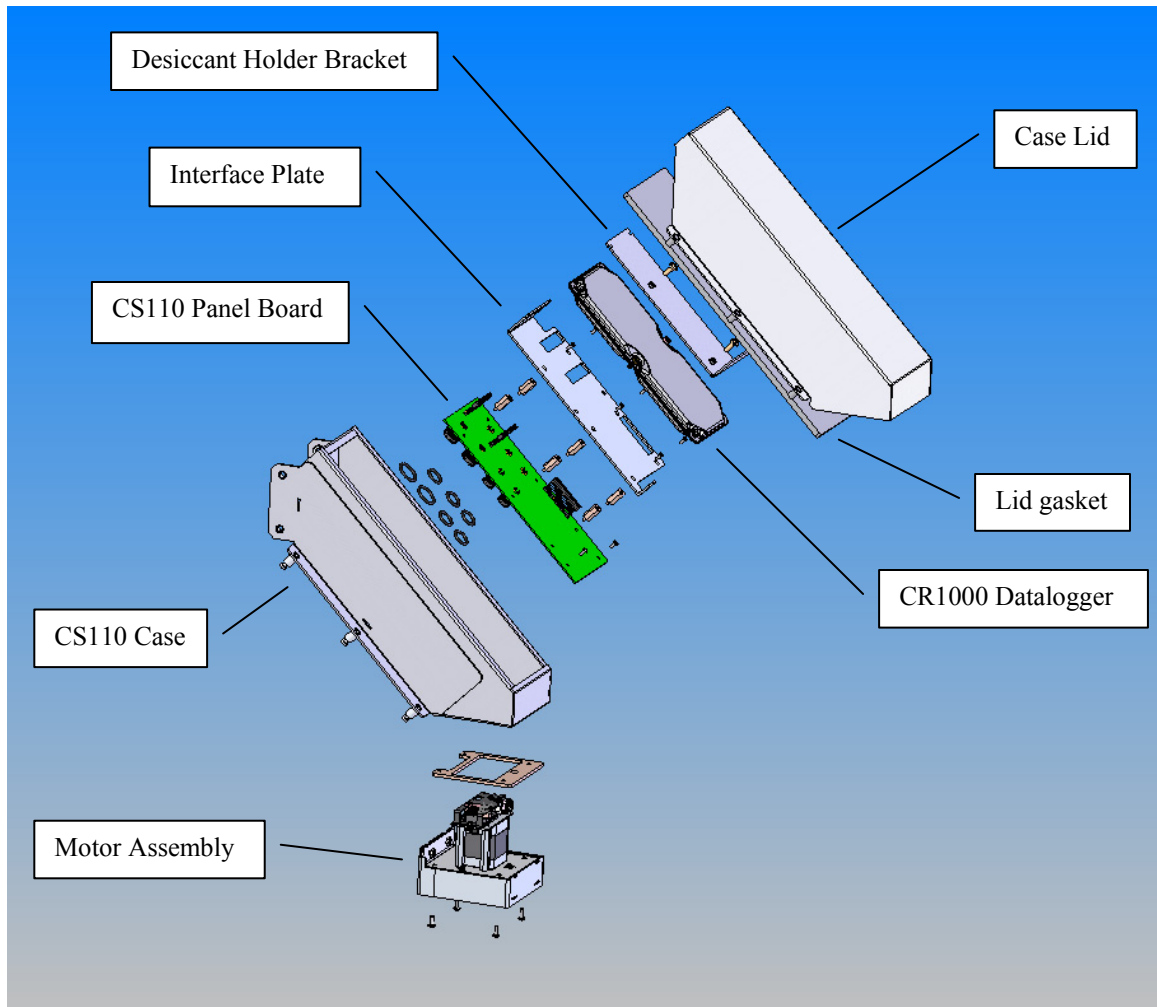


FIGURE D-1. Exploded view of CS110 Electric Field Meter

D.1 Lid Gasket

Whenever removing the CS110 case lid inspect the lid gasket for damage and replace (PN: 17533) in order to form a good seal.

D.2 Changing Out the CR1000

The CR1000 datalogger is accessible in the CS110 by removing the case lid. The CR1000 is secured to the CS110 via the desiccant holder bracket along with the two thumb screws on the CR1000 module. Light prying on the CR1000 module is required to unplug the three 40-pin connectors that interface to the

CS110 panel board, after removing the two thumb screws on the CR1000 module.

When installing a CR1000 into the CS110 case, first check for proper orientation of the three 40-pin connectors that interface to the CS110 panel board. Once proper connector orientation is verified, set the CR1000 into the CS110 case and feel for proper positioning of the three 40-pin connectors. When the connector shrouds are engaged, press down firmly on the CR1000 to mate the connector pins, prior to engaging the two thumb screws on the CR1000 module. Replace the desiccant holder bracket and desiccant after tightening the thumb screws.

D.3 Changing Out Motor Assembly

First remove the CR1000 by removing the desiccant holder bracket along with the two thumb screws on the CR1000 module. Next remove the black anodized interface plate between the CR1000 and CS110 panel board. Unplug the three locking electrical connectors on the CS110 panel board from the motor assembly.

Remove the stator by loosening the 2 Philips head screws located on the underside of the CS110. Next remove the four Philips head screws that attach the motor assembly to the white powder-coated aluminum case. With the four screws removed, carefully break it free from the bond to the gasket and allow it to be removed through the bottom of the CS110 case. Be sure to check the integrity of the motor assembly gasket on the CS110 case before replacing the motor assembly.

NOTE

Replacement of the motor assembly invalidates the factory calibration of a CS110 because of possible dimensional differences between assemblies.

D.4 Changing Out the CS110 Panel Board Assembly

First remove the CR1000 by removing the desiccant holder bracket along with the two thumb screw on the CR1000 module. Next remove the black anodized interface plate between the CR1000 and CS110 panel board.

Next remove the mounting posts that support the black anodized interface plate followed by the two Phillips head screws by the motor assembly that attach the CS110 panel board PCB to the CS110 case. Disconnect the three locking electrical connectors that connect signals between the CS110 panel board and the motor assembly. Next remove the plastic nuts from the circular connectors on the outside of the CS110 case. The CS110 panel board should now be free and can be maneuvered out of the case.

Reverse the above procedure when installing a CS110 panel board PCB. Make sure that the circular connectors each have a functional o-ring before placing the CS110 panel board inside the CS110 case. The plastic nuts on the circular connectors should be tightened to a torque of 10-12 inch-lbs.

Readers are referred to Section 10 on Maintenance for instructions on how to clean the CS110 electrodes and change desiccant in the sealed CS110 case.

D.5 Shutter/Encoder Alignment

A factory trim is done to align the position of the CS110 shutter with an Index mark on the rotary position encoder. Re-trimming of the shutter/encoder alignment becomes necessary after encoder disassembly. The procedure to trim the shutter/encoder alignment uses a CS110 single-step trim instruction called **CS110Trim**. This instruction allows a single shutter step open (flag 1) and closed (flag 2) utilizing the flag capability in LoggerNet. The following CS110 program listing (CS110_Index_Trim.cr1) is for trimming the Index mark to the fully closed shutter position.

```
'CS110 program to trim index to fully closed shutter position (CS110_Index_Trim.cr1).
' Index/shutter trim procedure follows:
' 1. Take at least 8 full-steps open via flag(1) in order to synchronize
'   motor coils with motor controller phase state.
' 2. Open shutter to the fully opened position via flag(1) and flag(2).
' 3. Utilizing flag(3) drop into scan that fully closes shutter with 25 full steps.
' 4. Monitor index output on o-scope or voltmeter and trim encoder adjustment so that
'   Index = 5 V in fully closed position.
' 5. Take a step open (flag(1)) and then closed (flag(2)) and verify park on Index.
' Updated last by Jody Swenson on 7/15/04.

Public Flag(3)
Public I
Public Battery
Public Panel_Temp

BeginProg

Scan(10,msec,0,0)
  If Flag(1) Then
    CS110Trim(1)           'Take a step open.
    Flag(1) = 0           'Reset Flag 1.
  EndIf
  If Flag(2) Then
    CS110Trim(-1)        'Take a step closed.
    Flag(2) = 0           'Reset Flag 2.
  EndIf
  If Flag(3) Then        'Exit scan via Flag 3.
    Flag(3) = 0
    ExitScan
  EndIf
NextScan

Scan(1000,msec,0,0)
  For I = 1 To 25        'Loop to fully close a fully opened shutter.
    CS110Trim(-1)        'Take a step closed.
    Delay (0,10,mSec)
  Next I
ExitScan
NextScan

Scan(10,msec,0,0)
  If Flag(1) Then
    CS110Trim(1)           'Take a step open.
    Flag(1) = 0           'Reset Flag 1.
```

```
EndIf
If Flag(2) Then
  CS110Trim(-1)           'Take a step closed.
  Flag(2) = 0           'Reset Flag 2.
EndIf
NextScan
EndProg
```

The CS110_Index_Trim.cr1 program uses flags 1, 2 and 3 available in LoggerNet, for user control. Flags 1 and 2 are used to single step the shutter one step open and closed, respectively. These flags are used initially to position the shutter into the fully opened position, as observed visually by stator to shutter overlap.

NOTE

At least 8 consecutive open (flag 1) initiated motor steps should occur prior to arriving at the fully open position in order to guarantee synchronization between the motor controller phase state and the stepper-motor coils being energized.

Stator to shutter overlap exists in the fully opened and fully closed positions so that slight shutter position variations do not alter the measured result. A fully opened shutter will display symmetrical stator to shutter overlap, within the 1.8° stepper motor step size, on both edges of each of the 4 openings in the stator.

Once the shutter has been adjusted to the fully open position by means of flags 1 and 2, flag 3 is to be set high to execute a 25 closed step loop, which positions the shutter in the fully closed position, which is the desired position for the Index trim. No visible gaps between the stator and shutter blades should be visible in the fully closed shutter position. Once in the fully closed position, hook an oscilloscope or dc voltmeter to the **Index** test pin on the CS110 panel PCB. The Ports and Flags button on the LoggerNet connect screen along with a graphical display can also be used for trimming if the update interval is set to 50 ms.

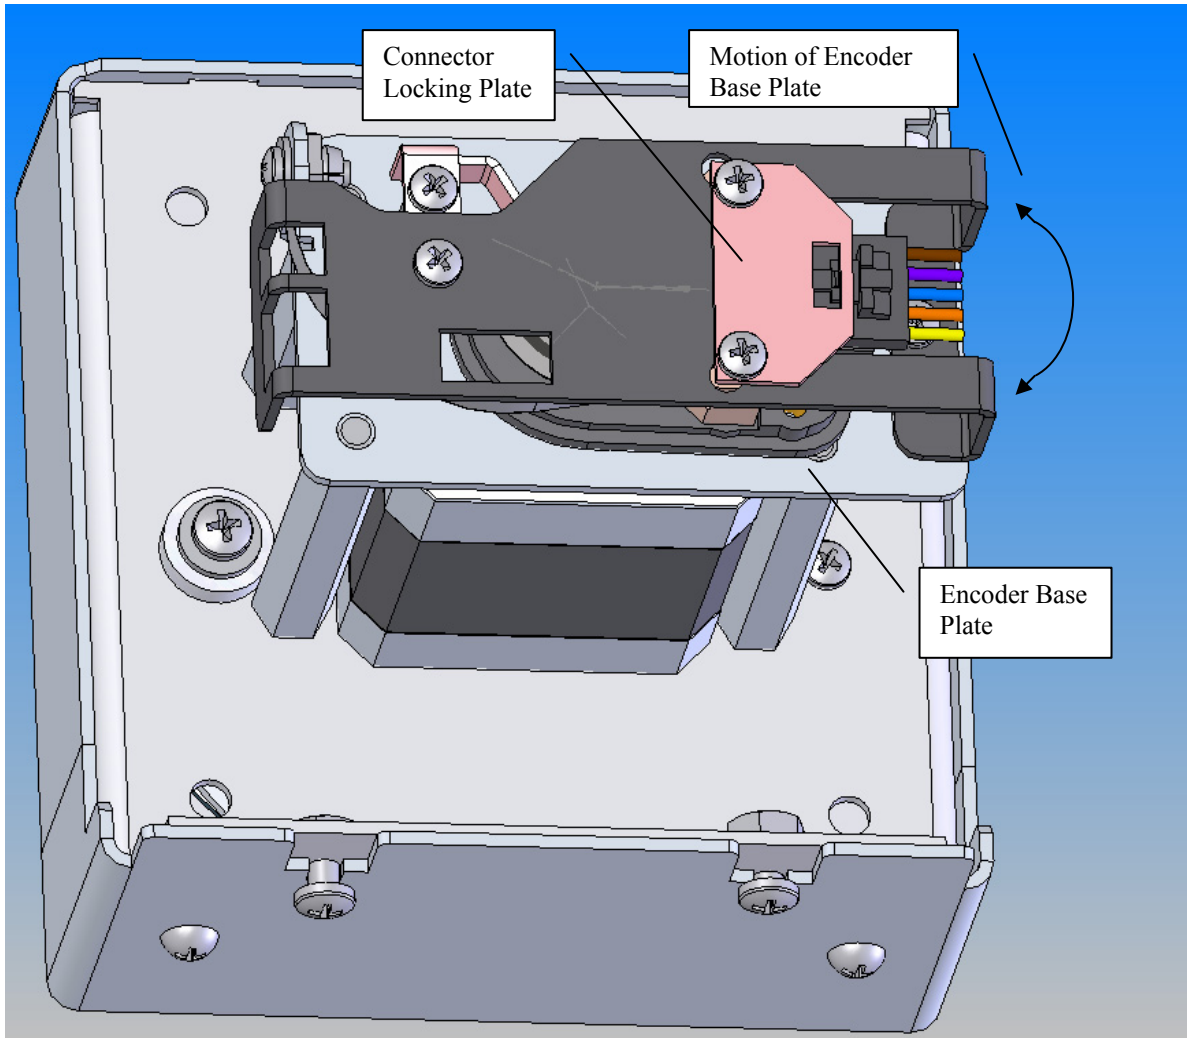


FIGURE D-2. CS110 motor assembly

Referring to Figure D-2, loosen the 2 Philips head screws on the connector locking plate on the top of the motor assembly. Slowly rotate the encoder base plate until Index (Control Port # 8) always equals 5 V (5 V = True = Green in LoggerNet). Tighten down the 2 Philips head screws on the connector locking plate and verify that Index still equals 5 V. Using flags 1 and 2, move the motor a step away from and then back to the fully closed position and verify that Index equals 5 V for the fully closed position.

The **CS110Shutter** instruction can be used to open, pause and then close the CS110 shutter to allow visual inspection/verification of proper opened and closed shutter positions. The following CS110 program can be used to verify proper opening and closing of the shutter. Stator to shutter overlap exists in the fully opened and fully closed positions so that slight shutter position variations do not alter the exposed area to the sense electrode. A fully opened shutter will display symmetrical stator to shutter overlap, within the 1.8° stepper motor step size, on both edges of each of the 4 openings in the stator. No visible gaps between the stator and shutter blades should be visible on a fully closed shutter.

```

'Program to open/close the CS110 shutter (CS110_Shutter1.cr1).
'Last updated by Jody Swenson on 9/26/05.

Public PTemp
Public Batt
Public stat(2)

DataTable(Efield,1,-1)
  Sample(2,stat,FP2)
  Sample(1,PTemp,IEEE4)
  Sample(1,Batt,IEEE4)
EndTable

BeginProg

  Scan(5000,msec,0,0)
  PanelTemp(PTemp,250)
  Battery(Batt)
  CS110Shutter(stat(1),1)           'Fully open shutter.
  Delay (0,3000,mSec)
  CS110Shutter(stat(2),0)         'Fully close shutter.
  CallTable Efield
  NextScan
EndProg

```

D.6 Motor O-ring Seal

A double-seal O-ring is located on the motor shaft underneath the CS110 shutter to help seal the CS110 case. Use Allen head screw-driver (PN: 17531) to remove the 1st set screw and loosen the second (primary) set screw in the shutter hub, in order to access and replace the motor O-ring. The motor O-ring slides on a UHMW washer for reduced friction and wear.

Apply a thin layer of Parker Super O-lube silicone base grease to PN 21759 O-ring. Wipe off excess. Install PN 21759 O-ring on shaft. Clean excess grease off the shaft. After replacing the motor O-ring, the CS110 shutter is installed to compress the O-ring. When replacing the shutter, line up the set screw hole so that it is perpendicular to the flat surface on the motor shaft. The shutter should then be compressed by applying a precise force. Campbell Scientific part number TLS16061 is used to apply the precise force. A second shutter hub set screw is used to prevent the primary shutter hub set screw from working loose during operation.

NOTE

Removal and replacement of the shutter from the motor shaft necessitates a check and possibly re-trimming of the Index to the fully closed position as described in Shutter/Encoder alignment. Removal and replacement of the shutter also invalidates the factory calibration because of possible dimensional differences when reassembled.

Appendix E. CS110 as a Slow Antenna

As previously mentioned the CS110 can sample the external electric field at a maximum rate of 5 Hz (200 ms) using the **CS110** instruction. Faster sampling of the rapid electric field changes associated with lightning discharges is desirable in some applications, and can be accomplished with the CS110 electric field meter configured as a Slow Antenna which is sometimes called a field change meter.

E.1 Response of the CS110 Slow Antenna in the Frequency Domain

The CS110 as a Slow Antenna with the 250 μ s integration responds to events as shown in Figure E-1. The lower frequency limit is due to the measurement circuitry and the upper frequency limit is a function of the integration time. Both are explained below.

The **CS110Shutter** instruction can be used to fully open the shutter, indefinitely exposing the sense electrode to external fields. Execution of the **CS110Shutter** instruction with the “open” command changes the CS110 panel board charge amplifier circuitry to a slow antenna by switching in a 200 M Ω resistor in parallel with the 330 pF feedback capacitor, resulting in a $(330\text{pF}) \cdot (200\text{M}\Omega) = 66$ ms decay time constant. In this slow antenna configuration the charge amplifier has a high-pass filter frequency response with the lower cutoff frequency defined by the decay time constant such that $f_{3\text{dB}} = (2 \cdot \pi \cdot R \cdot C)^{-1} = 2.4$ Hz. This means that events with frequencies higher than 2.4 Hz (shorter than 417 ms) are “passed through” while lower frequency events are “cut off” (search “cutoff frequency” in Wikipedia). The -3dB point for voltage is:

$$-3\text{dB} = \sqrt{10^{-3/10}} = 0.708 \text{ of true}$$

The CS110 can measure the slow antenna output at rates up to 50 Hz (100 Hz may be possible but it has not been tested), using the fast integration (250 μ s integration) for the **VoltDiff** instruction. Voltage measurements using the 250 μ s integration duration for the analog integrator, result in an upper 3 dB bandwidth of 1.8 kHz (0.555 ms). Figure E-1 shows the combined effect of both filters.

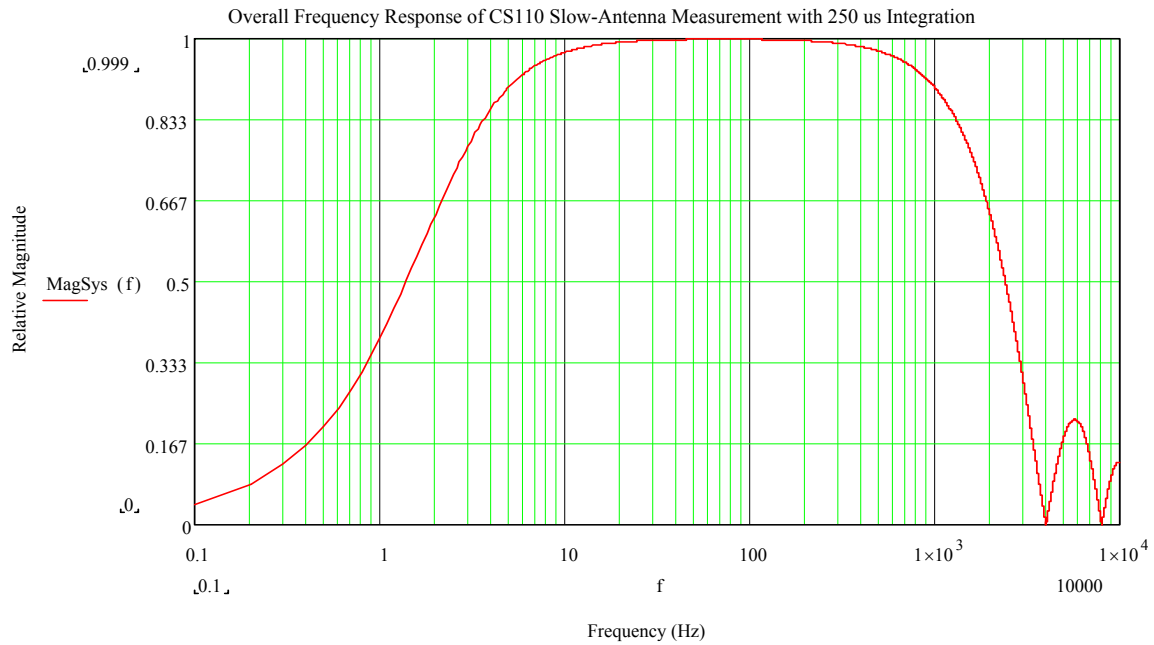


FIGURE E-1. CS110 slow antenna frequency response

E.2 Response of the CS110 Slow Antenna in the Time Domain

The following graphs shows one lightning strike measured at 50 Hz by both the CS110 slow antenna and by one of Kennedy Space Center's (KSC) field mills. In Figure E-3 the KSC electric field meter readings have been converted to efield change per measurement.

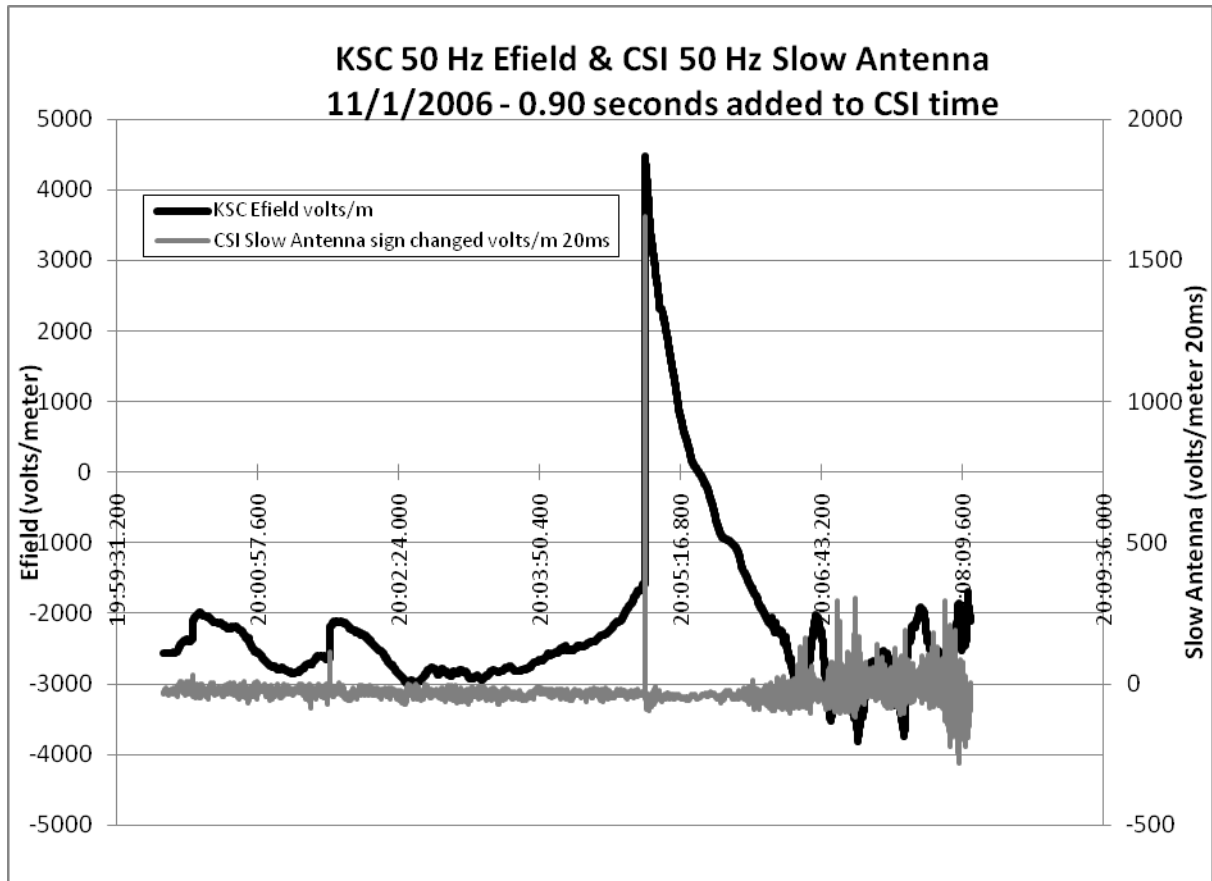


FIGURE E-2. KSC electric field and CS110 slow antenna data

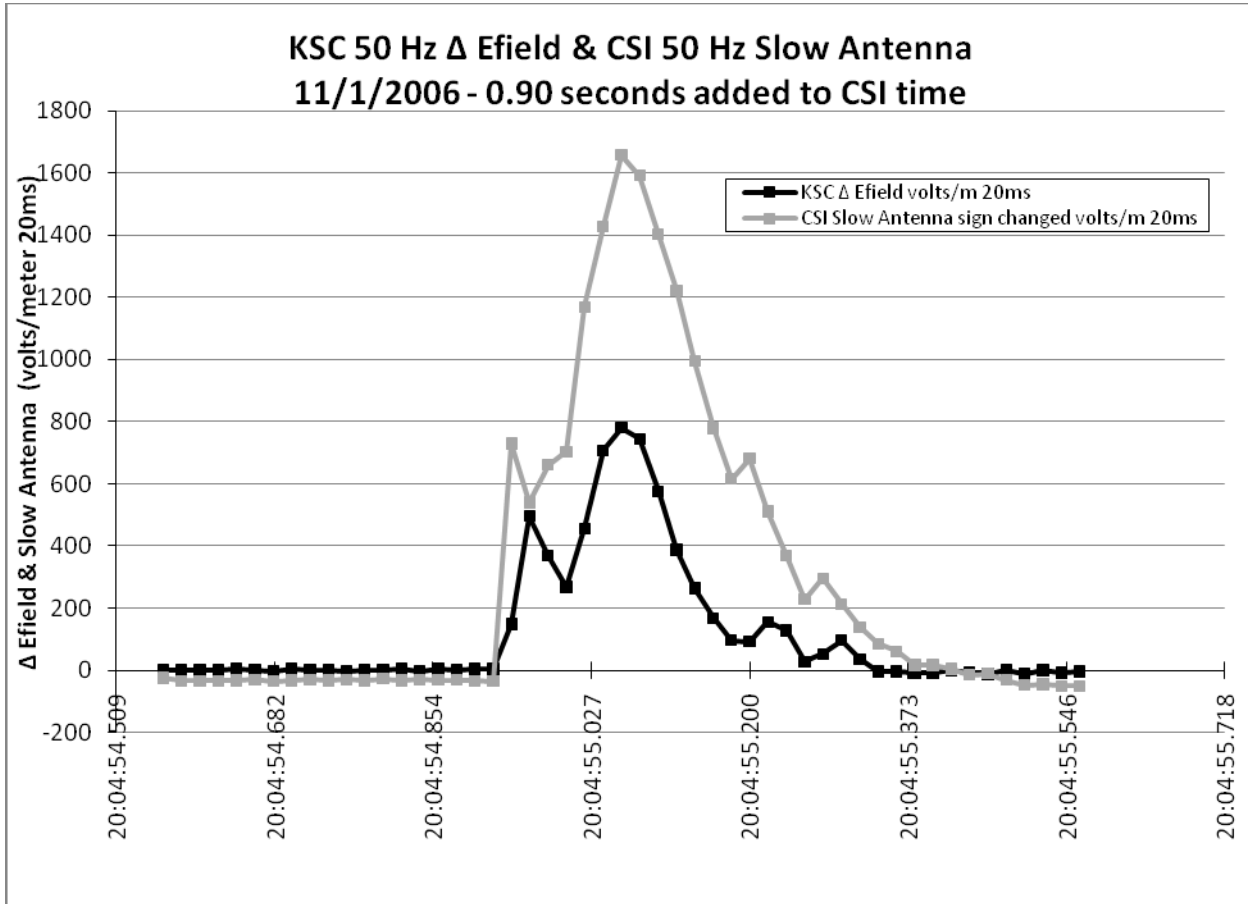


FIGURE E-3. KSC electric field change and CS110 slow antenna data

The KSC electric field mill and the CS110 were not precisely synced accounting for some of the differences in the data shown in the above graph. Since that time, the CS110 has been improved and now has the ability to sync to within $\pm 10 \mu\text{s}$ of the GPS signal's PPS pulse. The resolution of accuracy for the clock set is 10 microseconds if the internal CR1000 datalogger has a hardware revision number greater than 007 (RevBoard field in the datalogger's Status table).

E.3 Programming

The following CRBasic program utilizes the slow antenna capability of the CS110.

```
'Program to use the CS110 in slow antenna mode (slowant1.crl).
'Last updated by Jody Swenson on 9/30/05.
PipeLineMode

Const Mult = 85
Public Delta_E
Public Delta_E_mV2500
Public stat(2)
Public E_field
Public Leakage

DataTable(SlowAnt,1,-1)
    Sample(1,Delta_E,IEEE4)
EndTable

BeginProg
    CS110 (E_field,Leakage,stat(1),250,Mult,0)           'Measure E_field and leakage.
    CS110Shutter(stat(2),1)                             'Fully open shutter.
    Scan(20,msec,0,0)
        VoltDiff (Delta_E,1,mV250,8,False,0,250,Mult,0) 'no input reversal.
        VoltDiff (Delta_E_mV2500,1,mV2500,8,False,0,250,Mult,0) 'no input reversal.
        If Delta_E = NAN Then
            Delta_E = Delta_E_mV2500
        EndIf
        CallTable SlowAnt
    NextScan
EndProg
```

In the above program the **PipeLineMode** instruction enables parallel task processing necessary to complete a scan in 20 ms. The **CS110** instruction following the **BeginProg** statement provides a measure of the absolute electric field along with a leakage current compensation value, and is only executed once. The **CS110Shutter** instruction can fully open or fully close the shutter, based on the whether the 2nd parameter is a 1, or 0, respectively. Two **VoltDiff** instructions are used on two different input voltage ranges to provide more dynamic range in the charge amplifier output measurement.

The CS110 can be programmed to operate as a field meter and then switch to operate as a slow antenna. For example, efield measurements may be desired until they exceed an alarm threshold of ± 1500 V/m after which slow antenna (field change) measurements may be desired. The CR1000 operating system does not allow the **Sequential Mode** command and the **Pipeline Mode** command used in the above example to exist in the same program. For the CS110 to be able to switch between measuring the electric field with the CS110 instruction and the electric field change in the “slow antenna” mode, the slow antenna instructions must be run in the **Sequential Mode**. One way to accomplish this would be to program the CR1000 to monitor a 1 minute running average of the efield and when it exceeds ± 1500 v/m switch to the slow antenna mode for a fixed amount of time and then return to the field meter mode.

E.4 Calibration

The factory calibration described in Section 5 applies to the maximum amplitude of the step response of the CS110 when it is operating as a slow antenna. Switching in the 200 M Ω resistor in the feedback path simply slows the decay of the signal induced on the sense electrode resulting in a 66 millisecond decay time constant

The CS110 operating as a slow antenna returns the change in the electric field with units of volts per meter per scan. A 50 Hz scan interval would yield:
X volts * meter⁻¹ * 20 ms⁻¹.

Appendix F. Example CRBasic Programs

An example CS110 weather station program using a variable electric field measurement rate in order to minimize current consumption in solar powered applications follows.

```
'CS110 efield and weather station program with variable measurement
'rate for low-power consumption.(CS110_low_power.cr1).
'Measures rainfall, wind speed and direction, solar radiation,
'relative humidity, air temperature, and electric field.
'Updated last by Jody Swenson on 9/18/04 for Mparallel_plate and Csite.

const Mparallel_plate = 85
const Csite = 0.10
const Mcorrected = Mparallel_plate* Csite
const SLOW_INTERVAL = 10
const FAST_INTERVAL = 1

Public E_field
Units E_field=volts/m
Public battery_volt
Public leakage_cur
Units leakage_cur=nA
Public status
Public panel_temp
Units panel_temp=DegF
Public rain_fall
Units rain_fall=inch
Public wind_speed
Units wind_speed=mph
Public wind_dir
Units wind_dir=deg
Public solar_rad
Units solar_rad=W/m2
Public air_temp
Units air_temp=DegF
Public RH
Units RH=%
Public internal_RH
Units internal_RH=%

Public count
Public E_field_int
Public run_avg10
Public abs_run_avg600

Public E_status(16)
Public k
Public meas_error
```

*'Approximate value for weather station site.
'Mcorrected is multiplier for CS110 instruction.*

'Interval to make efield measurement rate

*'Efield status array.
'Index for E_stat array.
'Disable variable for slow table.*

```

DataTable(Tabslow,1,-1)                                '-1 to auto-allocate all available memory.
  DataInterval(0,60,sec,10)                             'Averaged 60 second output data.
  Average(1,E_field,iieee4,meas_error)
  Sample (1,run_Avg10,iieee4)
  Totalize (16,E_status,FP2,0)                          'Look at Efield status array for last 60 seconds.
  Average (1,leakage_cur,FP2,0)
  Average(1,panel_temp,FP2,0)
  Totalize (1,rain_fall,FP2,0)
  WindVector (1,wind_speed,wind_dir,FP2,False,0,0,0)
  Average (1,solar_rad,FP2,0)
  Average(1,air_temp,FP2,0)
  Average (1,RH,FP2,0)
  Average (1,battery_volt,FP2,0)
  Average (1,internal_RH,FP2,0)
EndTable

DataTable(Tabfast,1,-1)                                '-1 to auto-allocate all available memory.
  Sample(1,E_field,iieee4)
  Sample (1,run_Avg10,iieee4)
  Sample (1,status,FP2)
  Sample (1,leakage_cur,FP2)
  Sample (1,rain_fall,FP2)
  Sample (1,wind_speed,FP2)
  Sample (1,wind_dir,FP2)
  Sample (1,solar_rad,FP2)
  Sample (1,air_temp,FP2)
  Sample (1,RH,FP2)
  Sample (1,battery_volt,FP2)
EndTable

BeginProg
  E_field_int = FAST_INTERVAL                          'Initialize to fast interval.
  Scan(1,sec,0,0)
    for k = 1 to 16                                    'Initialize status array.
      E_status(k) = 0
    next
  PanelTemp (panel_temp,250)
  panel_temp = panel_temp*1.8 + 32                    'Convert to Fahrenheit.
  Battery (battery_volt)
  VoltDiff (internal_RH,1,mV2500,5,True ,0,250,0.1,0)
  PulseCount (rain_fall,1,2,2,0,0.01,0)              'TE525 tipping bucket 0.01 inches per tip.
  PulseCount (wind_speed,1,1 ,1,1,0.2192,0)          'Mult for 05103 Wind Monitor.
  BrHalf (wind_dir,1,mV2500,4,Vx2,1,2500,False,450,250,355,0) 'Mult. for 05103 Wind Monitor.
  VoltDiff (solar_rad,1,mV7_5,3,True,450,250,200,0)
  SW12 (1 )                                           'Apply switched 12 V power to the probe.
  Delay (0,150,mSec)                                  'Warm up probe before measurements.
  VoltSe (RH,1,mV2500,1,1,0,250,0.1,0)
  VoltSe (air_temp,1,mV2500,2,1,0,250,-18,-40)
  SW12 (0)                                             'Turn off power to the probe.
  if RH > 100 and RH < 108 then
    RH = 100
  Endif
  count = count + 1
  if (count >= E_field_int) then
    count = 0                                          'reset the count for SLOW_INTERVAL
    meas_error = 0                                    'Initialize disable variable for Efield average in slow table.

```

```

CS110(E_field,leakage_cur,status,_60Hz,Mcorrected,0)
If E_field = NAN Then
    meas_error = 1           'Disable output to slow table if efield = NAN.'
    E_field_int = FAST_INTERVAL 'Go to fast interval if NAN.'
EndIf
E_status(status) = 1       'Set appropriate element in status array.'
Endif
If E_field <> NAN Then
    AvgRun (run_avg10,1,E_field,10) 'Used for average output in fast table.'
    AvgRun (abs_run_avg600,1,ABS(E_field),600) 'Used to stay longer at fast interval.'
EndIf
if (E_field>100 or ABS(E_field)>=300 or abs_run_avg600>=300)and (battery_volt>11.0) then
    E_field_int = FAST_INTERVAL
else
    E_field_int = SLOW_INTERVAL
EndIf
If E_field_int = FAST_INTERVAL Then
    CallTable Tabfast 'Only call fast table when fast efield active'
EndIf
CallTable Tabslow 'Call slow every time at slow interval.'
NextScan
EndProg

```

In the above program all measurements, except the electric field measurement, are done once per second. The electric field measurement is done once every SLOW_INTERVAL when measured electric field values are between -300 V/m and +100 V/m as determined by an **if** statement. The -300 V/m and +100 V/m values are somewhat arbitrary and can easily be changed to better suit a given application. When measured electric field values fall outside of the -300 V/m and +100 V/m range, the electric field measurement rate becomes the FAST_INTERVAL. A running average instruction (**AvgRun**) is used to maintain measurements at the FAST_INTERVAL for some time following elevated electric fields, even after several near zero measurements.

Appendix G. CS110 2 Meter CM10 Tripod Site



FIGURE G-1. CS110 2 Meter CM10 Tripod site

The Tripod_CS110 site consists of the CS110 mounted on the CM10 Tripod at a height of 2 meters, and a 12 x 14 inch enclosure.

The following may affect the site calibration factor, Csite:

- CM10 Tripod
- CS110 Electric Field Meter
- ENC 12/14 Enclosure

If the above items are installed using the following set of instructions, the site is level with a 25 foot (762 cm) radius of gravel around the tripod and there are no obstructions higher than 18 degrees from the center of a measurement site² then the Csite determined for this configuration should be valid.

Installation of the Tripod_CS110 Site:

Drive the ground rod into the ground where the center of the tripod is to be placed.

Extend the tripod legs so the far end of the sliding clamp is 56 inches (142 cm) from the mast end of the pipe. Extending the legs as described above puts the feet on a circle with a radius of approximately 77 inches (196 cm) from the center of the tripod to the outside edge of the pivoting feet. The distance from the top of the top collar to the ground will be approximately 40 inches (102 cm). Locate the center of the tripod above the ground rod with one leg of the tripod pointing toward the equator. Level the tripod by removing or adding small amounts of gravel under the feet as needed.

Apply Teflon tape to both ends of the 1 ¼ inch (3.175 cm) outside diameter mast.

Attach the cap to the top of the mast.

Attach the CS110 mounting bracket to the mast with the top of the bracket about 9¼ inches (23.5 cm) below the top of the cap on the mast but don't tighten bolts very tight as it will likely need to be rotated and either raised or lowered slightly.

Mount the completed mast on the tripod.

Adjust the CS110 mounting bracket so the top of the mounting bracket is approximately 90 inches (229 cm) above the ground and between the two legs opposite the equator still leaving the bolts not too tight yet. Mount the CS110 on the mounting bracket. The field meter should now be facing away from the equator with the face of the stator 78 ¾ inches or 200 cm above the ground. Tighten the mounting bolts. See Figure G-2.



FIGURE G-2. CS110 on CM10 Tripod Mast

Mount the fiberglass enclosure to the top of the leg facing the equator with the top bracket approximately 2 inches (5 cm) below the top of the leg. Be careful opening the lid because in this almost horizontal position it is possible to pull the hinge rivets out of the enclosure.

If there is a solar panel, install the solar panel on the leg facing the equator below the enclosure. Tilt the solar panel at an angle less than horizontal that is equal to the latitude plus 10 degrees (see solar panel manual).

Ground the CS110 Electric Field Meter (Figure G-2), the tripod, and the battery (through the enclosure ground) with three separate ground wires as shown in Figure G-3. Power and communication cables should be run down the equator side of the mast and under the enclosure as shown. Wire-tie all cables into place so they don't move with the wind.



FIGURE G-3. Earth grounding

Stake the tripod to the ground and/or weigh it down with sand bags.


Determination of Csite

Surface mounted upward facing CS110: SN1022 with $M_{parallel_plate} = 87.6$

Tripod with CS110 only: SN1023 with $M_{parallel_plate} = 81.77$

Each CS110 recorded one minute averages of 1 second measurements of electric field data for the same 2200 to 2300 hour time period on October 2, 2005. The data from both units is plotted in Figure G-4. A best-fit line was computed. The linear regression yields a $C_{site} = 0.105$ for the Tripod CS110 Only Site.

Site Correction for Tripod CS110 Only Site - October 2, 2005
 1 minute average of 1 second data
 Results indicate Csite = 0.105.

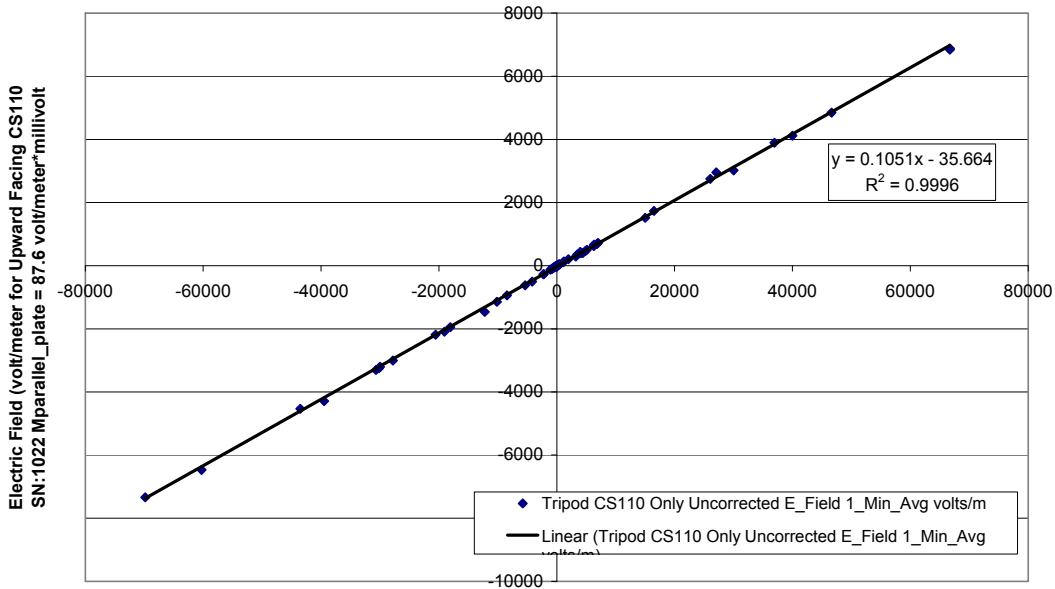

Uncorrected (Csite = 1) Electric Field (volt/meter) for Tripod CS110 Only site
 SN: 1023 Mparallel_Plate = 81.77 volt/meter*millivolt

FIGURE G-4. Determination of Csite

Appendix H. Tripod CS110 and StrikeGuard Site

H.1 Tripod CS110 and StrikeGuard



FIGURE H-1. Tripod CS110 and StrikeGuard

The Tripod CS110 and StrikeGuard Site includes the following that affect Csite:

- CM10 Tripod
- StrikeGuard Lightning Detector
- CS110 Electric Field Meter
- ENC 12/14 Enclosure

If the above items are installed using the following set of instructions, the site is level with a 25 foot radius of gravel around the tripod and there are no obstructions higher than 18 degrees from the center of a measurement site² then the Csite determined for this configuration should be valid.

H.1.1 Installation of the Tripod CS110 and StrikeGuard Site

Drive the ground rod into the ground where the center of the tripod is to be placed.

Extend the tripod legs so the far end of the sliding clamp is 56 inches (142 cm) from the mast end of the pipe. Extending the legs as described above puts the feet on a circle with a radius of approximately 77 inches (196 cm) from the center of the tripod to the outside edge of the pivoting feet. The distance from the top of the top collar to the ground will be approximately 40 inches (102 cm). Locate the center of the tripod above the ground rod with one leg of the tripod pointing toward the equator. Level the tripod by removing or adding small amounts of gravel under the feet as needed.

Apply Teflon tape to both ends of the 1 ¼ inch (3.175 cm) outside diameter mast.

Attach the cap to the top end of the mast.

Attach the CS110 mounting bracket to the mast with the top of the bracket about 9¼ inches (23.5 cm) below the top of the cap on the mast but don't tighten bolts very tight as it will likely need to be rotated and either raised or lowered slightly.

Mount the completed mast and cross arm on the tripod.

Adjust the CS110 mounting bracket so the top of the mounting bracket is approximately 90 inches (229 cm) above the ground and between the two legs opposite the equator still leaving the bolts not too tight yet. Mount the CS110 on the mounting bracket. The field meter should now be facing away from the equator with the face of the stator 78 ¾ inches or 200 cm above the ground. Tighten the mounting bolts. See Figure H-2.

Mount the StrikeGuard Lightning Detector to the top of the mast on the equator side of the mast with the top of the mounting bracket butted up against the cap on the top of the mast.



FIGURE H-2. CS110 and StrikeGuard on tripod mast

Mount the fiberglass enclosure to the top of the leg facing the equator with the top bracket approximately 2 inches (5 cm) below the top of the leg. Be careful opening the lid because in this almost horizontal position it is possible to pull the hinge rivets out of the enclosure.

If there is a solar panel, install the solar panel on the leg facing the equator below the enclosure. Tilt the solar panel at an angle less than horizontal that is equal to the latitude plus 10 degrees (see solar panel manual).

Ground the CS110 Electric Field Meter (Figure H-3), the tripod, and the battery (through the enclosure ground) with three separate ground wires as shown in Figure H-4.



FIGURE H-3. Grounding the CS110 grounding strap



FIGURE H-4. Grounding the tripod and battery

Stake the tripod to the ground or weight it down with sand bags.

Connect power and communication cables as shown in Figure H-5.

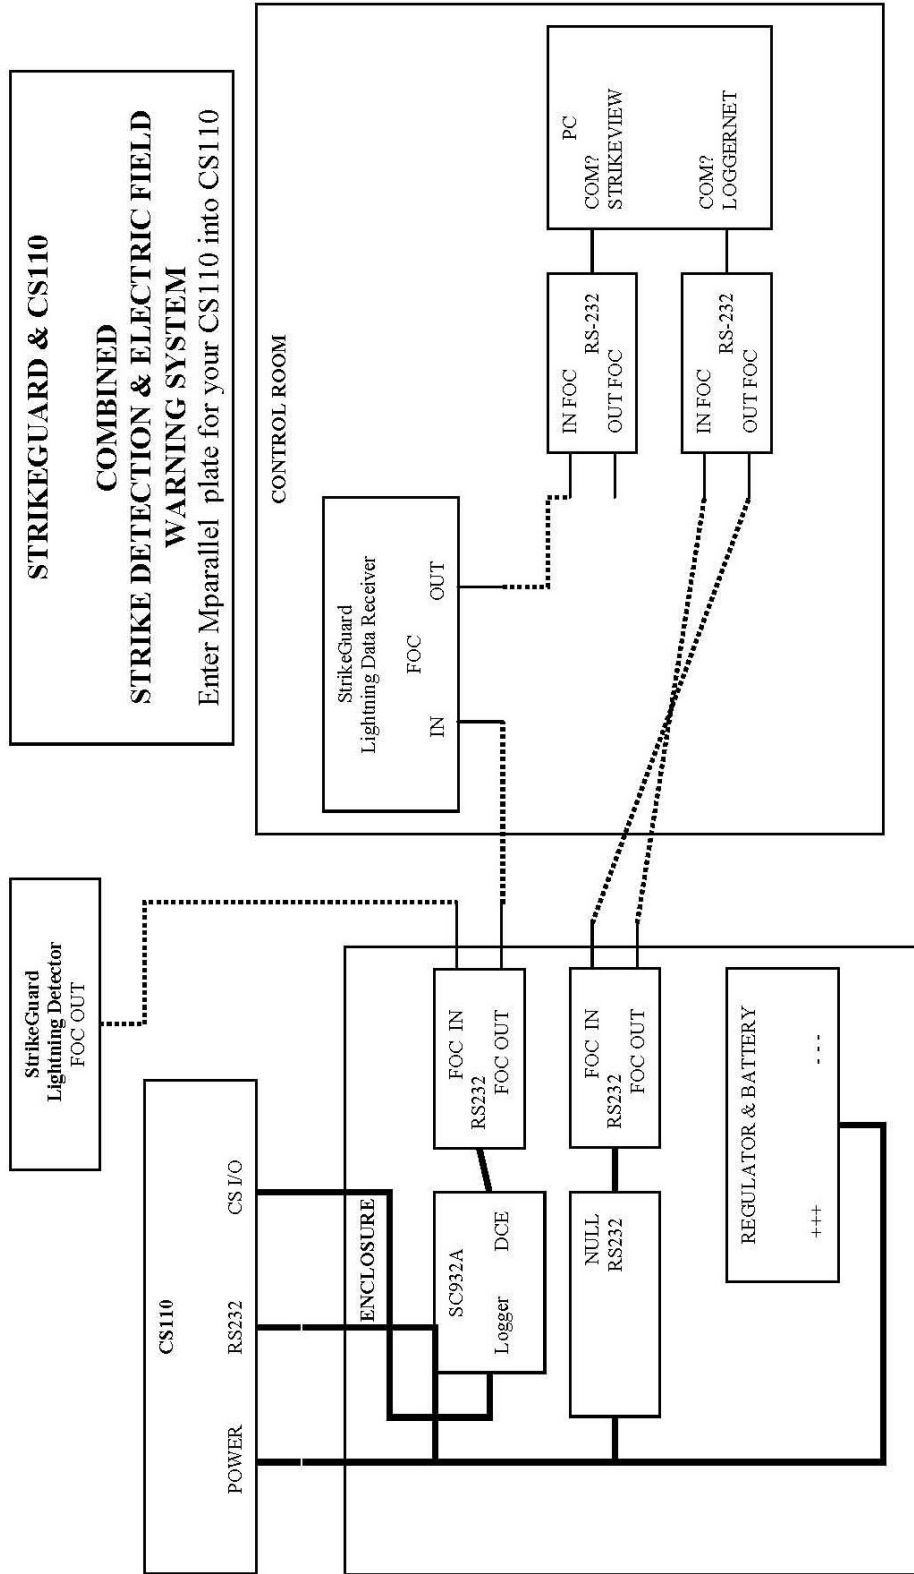


FIGURE H-5. Connections for combined system

Power and communication cables should be run down the equator side of the mast and under the enclosure as shown. Wire-tie all cables into place so they don't move with the wind.

H.1.2 Determination of Csite

Surface mounted upward facing CS110: SN1022 with $M_{parallel_plate} = 88.31$.

CM10 Tripod Mounted StrikeGuard and CS110: SN1023 with $M_{parallel_plate} = 81.77$.

Each CS110 recorded one minute averages of 1 second measurements of electric field data for the same one hour time period from 3 AM to 4 AM on August 11, 2005. The data from both units is plotted in Figure H-6. A best-fit line was computed. The linear regression yields a $C_{site} = 0.108$ for the Tripod CS110 and StrikeGuard Site.

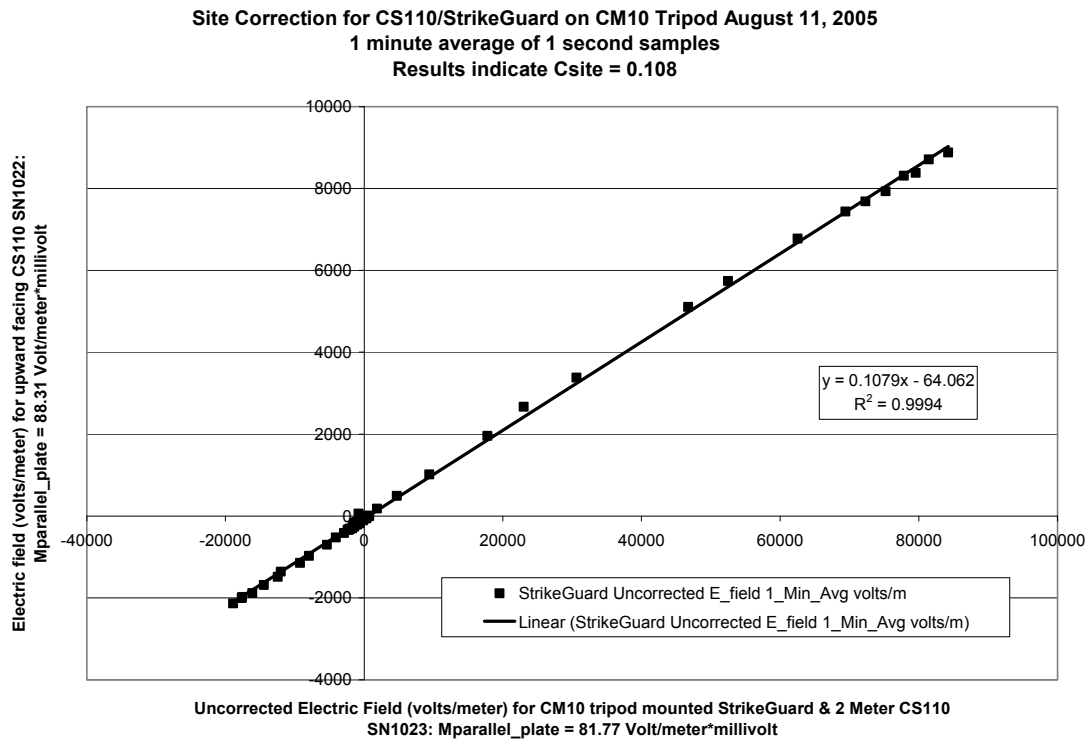


FIGURE H-6. Determination of Csite

Campbell Scientific Companies

Campbell Scientific, Inc. (CSI)

815 West 1800 North
Logan, Utah 84321
UNITED STATES
www.campbellsci.com • info@campbellsci.com

Campbell Scientific Africa Pty. Ltd. (CSAf)

PO Box 2450
Somerset West 7129
SOUTH AFRICA
www.csafrica.co.za • cleroux@csafrica.co.za

Campbell Scientific Australia Pty. Ltd. (CSA)

PO Box 8108
Garbutt Post Shop QLD 4814
AUSTRALIA
www.campbellsci.com.au • info@campbellsci.com.au

Campbell Scientific do Brazil Ltda. (CSB)

Rua Luisa Crapsi Orsi, 15 Butantã
CEP: 005543-000 São Paulo SP BRAZIL
www.campbellsci.com.br • suporte@campbellsci.com.br

Campbell Scientific Canada Corp. (CSC)

11564 - 149th Street NW
Edmonton, Alberta T5M 1W7
CANADA
www.campbellsci.ca • dataloggers@campbellsci.ca

Campbell Scientific Centro Caribe S.A. (CSCC)

300 N Cementerio, Edificio Breller
Santo Domingo, Heredia 40305
COSTA RICA
www.campbellsci.cc • info@campbellsci.cc

Campbell Scientific Ltd. (CSL)

Campbell Park
80 Hathern Road
Shepshed, Loughborough LE12 9GX
UNITED KINGDOM
www.campbellsci.co.uk • sales@campbellsci.co.uk

Campbell Scientific Ltd. (France)

3 Avenue de la Division Leclerc
92160 ANTONY
FRANCE
www.campbellsci.fr • info@campbellsci.fr

Campbell Scientific Spain, S. L.

Avda. Pompeu Fabra 7-9, local 1
08024 Barcelona
SPAIN
www.campbellsci.es • info@campbellsci.es

Please visit www.campbellsci.com to obtain contact information for your local US or International representative.