


Matching the Calibration Sheet Serial Number to the BaroVUE10 Serial Number

IMPORTANT: The calibration sheet supplied with your BaroVUE10 applies to the sensor card (BVC10). The serial number on the outside of the unit refers to the serial number of the BaroVUE10 Main Board. To confirm you have the correct calibration sheet, please open the device and check the serial number on the BVC10 sensor card itself.

Motherboard Serial Number



Sensor Card Serial Number

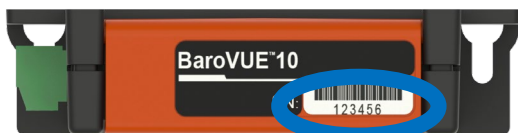

Certificate of Calibration

Instrument: BVC10 **Serial No:** 1001
Serial No: 1001
Manufacturer: Campbell Scientific Australia
Calibration ID: 6077df5f6e07e46e66c397c0

Instrument Calibration Condition
 As Found disposition: n/a
 As Left disposition: In tolerance

Recommended Calibration Schedule
 If the customer has not requested a calibration interval, a non-mandatory recommended interval is provided. Based on past experience and assumed normal usage, it is recommended that this instrument be calibrated in accordance with the interval stated below to ensure sustained accuracy and reliable performance.

Calibration date: 18-Apr-2021 at 11:02:17 Recommended Interval: 12 months

Calibration Standard Used
 This instrument has been calibrated against a Fluke7250i Pressure Controller/Calibrator standard. The 7250i is traceable to the National Institute of Standards and Technology (NIST, USA).

Make/Model	Serial Number	Cal. Due Date	Certificate Number
Fluke 7250i	69455	20 Jul 2021	1500288281

CSA certifies the above instrument meets or exceeds published specifications and has been calibrated using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology, an accepted value of a natural physical constant or a ratio calibration technique.

Document shall not be reproduced except in full, without the written approval of Campbell Scientific Australia.
 Page 1 of 2
 Campbell Scientific Australia. | 411 Bayswater Rd | Garbutt, QLD 4814 | +617 4401 7700 | www.campbellsci.com.au