


INSTRUCTION MANUAL



CM375 Portable 10-Meter Mast

Revision: 8/10

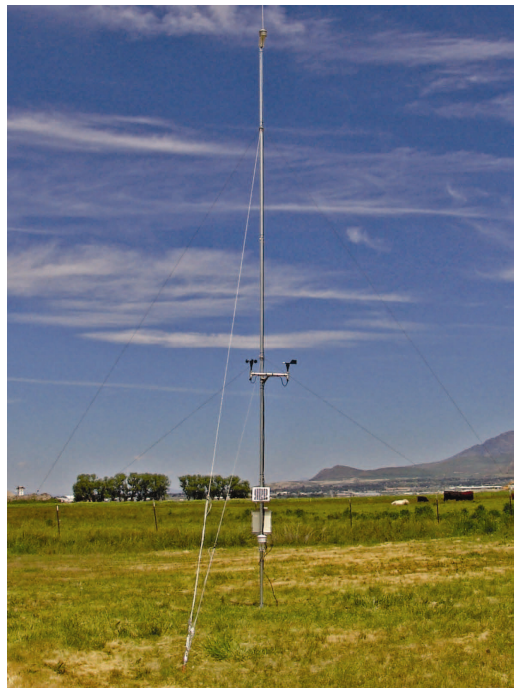

Copyright © 2009-2010
Campbell Scientific, Inc.

Warranty and Assistance

The **CM375 PORTABLE 10-METER MAST** is warranted by Campbell Scientific, Inc. to be free from defects in materials and workmanship under normal use and service for twelve (12) months from date of shipment unless specified otherwise. Batteries have no warranty. Campbell Scientific, Inc.'s obligation under this warranty is limited to repairing or replacing (at Campbell Scientific, Inc.'s option) defective products. The customer shall assume all costs of removing, reinstalling, and shipping defective products to Campbell Scientific, Inc. Campbell Scientific, Inc. will return such products by surface carrier prepaid. This warranty shall not apply to any Campbell Scientific, Inc. products which have been subjected to modification, misuse, neglect, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied, including warranties of merchantability or fitness for a particular purpose. Campbell Scientific, Inc. is not liable for special, indirect, incidental, or consequential damages.

Products may not be returned without prior authorization. The following contact information is for US and International customers residing in countries served by Campbell Scientific, Inc. directly. Affiliate companies handle repairs for customers within their territories. Please visit www.campbellsci.com to determine which Campbell Scientific company serves your country.

To obtain a Returned Materials Authorization (RMA), contact Campbell Scientific, Inc., phone (435) 753-2342. After an applications engineer determines the nature of the problem, an RMA number will be issued. Please write this number clearly on the outside of the shipping container. Campbell Scientific's shipping address is:

CAMPBELL SCIENTIFIC, INC.

RMA#_____

815 West 1800 North

Logan, Utah 84321-1784

For all returns, the customer must fill out a "Declaration of Hazardous Material and Decontamination" form and comply with the requirements specified in it. The form is available from our website at www.campbellsci.com/repair. A completed form must be either emailed to repair@campbellsci.com or faxed to 435-750-9579. Campbell Scientific will not process any returns until we receive this form. If the form is not received within three days of product receipt or is incomplete, the product will be returned to the customer at the customer's expense. Campbell Scientific reserves the right to refuse service on products that were exposed to contaminants that may cause health or safety concerns for our employees.

CM375 Table of Contents

PDF viewers note: These page numbers refer to the printed version of this document. Use the Adobe Acrobat® bookmarks tab for links to specific sections.

1. Overview	1
1.1 Specifications.....	1
1.2 Guy Duckbill Anchor Kits.....	2
2. CM375 Installation	3
2.1 Site Selection	3
2.2 Assembling Mast Sections.....	4
2.3 Lightning Rod Assembly and Mounting Instrumentation	12
2.4 Anchor Installation	13
2.5 Raise, Plumb Mast and Final Cable Tensioning	17
3. Maintenance	19

Figures

1-1. 21720 Tote	1
2.1-1. Assembled CM375	3
2.2-1. CM375 in Opened Tote.....	4
2.2-2. Mast Sections and Base.....	4
2.2-3. Mast Section 1 Oriented on Base	5
2.2-4. Spikes Installation	5
2.2-5. Coupler Installed in Top of Mast Section 1.....	6
2.2-6. Bag Containing Hardware.....	6
2.2-7. Mast Section 2 and Mast Section 3	7
2.2-8. Guy Ring, Mast Section 2 and Mast Section 3.....	7
2.2-9. 21663 Bottom Guy Kit.....	8
2.2-10. Guy Cable Inserted into Guy Ring	8
2.2-11. Mast Section 3 and Guy Ring/Collar Assembly.....	9
2.2-12. Mast Section 4 Ready to be Installed in Mast Section 3	9
2.2-13. Mast Section 5	10
2.2-14. Mast Section 5 Installed in Mast Section 4	10
2.2-15. 21661 Guy Kit.....	11
2.2-16. Mast Section 5 and Guy Ring/Collar Assembly.....	11
2.3-1. Lightning Rod Assembly.....	12
2.3-2. Installed Lightning Rod.....	12
2.4-1. Tape Measure in Slot for South Anchor.....	13
2.4-2. 19282 Duckbill Anchor and Cable Assembly (left). The 25699 has a threaded rod instead of the cable. The drive rod (right) is used for both the 19282 and 25699.....	13
2.4-3. Anchor Driven into Ground at 45° Angle	14
2.4-4. Locking Anchor.....	14
2.4-5. Tape Measure in Slot for North East Anchor.....	15
2.4-6. Turnbuckle Fastened to Guy Cable and Anchor	15
2.4-7. Top and Bottom Guy Cables Fastened to an Anchor	16

- 2.4-8. Rope Racket Assists Assembly..... 16
- 2.4-9. Adjusting Cable through Wedge Clamp..... 17
- 2.5-1. Raising the Mast 17
- 2.5-2. Pole Level Ensures Vertical Mast..... 18
- 2.5-3. Adjusting Turnbuckles 18
- 2.5-4. Guy Cables with 100 lbs of Tension..... 19

CM375 Portable 10-Meter Mast

1. Overview

The CM375 is a corrosion-resistant 30-ft (10 m) mast for applications requiring a tall yet portable instrument mount. It consists of five 6-ft (2 m) galvanized pipes, a stainless-steel base, guy cables, 1 m crossarm and mount, and grounding kit. Duckbill anchor kits (required) and a guy-wire tensioning kit (recommended) are ordered separately. All of the components fit inside an 80"-long bag allowing the CM375 to be carried from site to site (see Figure 1-1).



FIGURE 1-1. 21720 Tote

1.1 Specifications

Weight: 66 lbs (30 kg)

Mast: 30 ft (9.2 m) total length; consists of five 6-ft (1.82 m) sections

Main Mast Diameter: 1.9" (48.26 mm)

Top Section Mast Diameter: 1.74" (44.2 mm)

Base Radius: 20 ft (6 m) to each of three guy points, 120 degrees apart

Guy Configuration: three guy cables at two levels; guyed at 12 ft (3.6 m) and at 24 ft (7.2 m)

Recommended Guy Wire Pretension: 100 lbs each; check and adjust guy wire tension at least once a month, and after wind gusts exceeding 50 mph.

Maximum Weight of Mounted Equipment: 75 lbs (34 kg)

Maximum Allowable Wind Gust¹: 85 mph (136 km h⁻¹)

The wind gust value assumes:

- Proper installation
- Proper anchoring:
 - Adequate soil (guy anchors/base support)
 - Guy anchors at 20-ft from base with 120 degrees of separation
 - Proper guy tension (100 lbs each)
- No ice buildup
- Standard air quality or wind assessment configuration (see Table below)

¹ The amount of wind gust that this mount can withstand is affected by quality of anchoring and installation, guy wire tension, soil type, guy angle, and the number, type, and location of instruments fastened to the CM375.

Standard Air Quality Configuration		Standard Wind Assessment Configuration	
Height	Component	Height	Component
9.1 m	CM204 crossarm with a Wind Monitor and a 43502/43347 Aspirated Shield & RTD attached	9.1 m	Two CM202 crossarms with a 03101 Wind Sentry Anemometer attached to each crossarm
		8.5 m	CM202 with 03301 Wind Sentry Wind Vane attached
3 m	41003-5 Radiation Shield housing an HMP45C Temperature/RH Probe; Antenna; CM202 crossarm with a 43502/43347 Aspirated Shield & RTD attached	3 m	41003-5 Radiation Shield housing an HMP45C Temperature RH Probe; Antenna; CM202 crossarm with a 03101 Wind Sentry Anemometer attached
1.5 m	SP20 20-W Solar Panel	1.5 m	SP20 20-W Solar Panel
1 m	ENC16/18 Enclosure housing a CR1000 datalogger and PS100 Power Supply	1 m	ENC12/14 Enclosure housing a CR1000 datalogger and PS100 Power Supply

1.2 Guy Duckbill Anchor Kits

A choice of duckbill anchor kits is offered for the CM375. The 19282 Guy Duckbill Standard Anchor Kit is for standard soils, and the 25699 Guy Duckbill Heavy Duty Anchor Kit is for aggressive soils. Aggressive soils have:

- Resistivity of less than 3000 ohm-cm
- pH of less than 5
- Chloride of greater than 1000 ppm
- Sulfate of greater than 500 ppm
- Poor aeration

Both the 19282 and 25699 have one drive rod. The 19282 also has four duckbill anchors with a cable attached to each of them. At the end of the cable is a loop for connecting the guy wires. The 25699 has a threaded rod attached to each of the four duckbill anchors instead of the cable. At the end of the threaded rod is a metal ring for connecting the guy wires.

2. CM375 Installation

2.1 Site Selection

Select a site free from overhead power lines, and 100 feet (30 m) in any direction from trees, buildings and other obstructions (see Figure 2.1-1).



FIGURE 2.1-1. Assembled CM375

2.2 Assembling Mast Sections

Step 1: Remove mast sections and other bundled hardware from tote; unzip and loosen straps (see Figure 2.2-1).

NOTE Sections are numbered for sequential assembly (see Figure 2.2-2).



FIGURE 2.2-1. CM375 in Opened Tote

PN 21669 crossarm-to-pole mounting kit contains the lightning rod, copper grounding rod, and duckbill anchor drive rod.

Base



FIGURE 2.2-2. Mast Sections and Base

Step 2: Place Section 1 at deployment location with base oriented, as shown in Figure 2.2-3 and mast pointing NORTH.

NOTE

A compass is included in the optional "Tensioning Kit" for your use.



FIGURE 2.2-3. Mast Section 1 Oriented on Base

Step 3: Use spikes provided (3 each) to anchor base to site (see Figure 2.2-4).

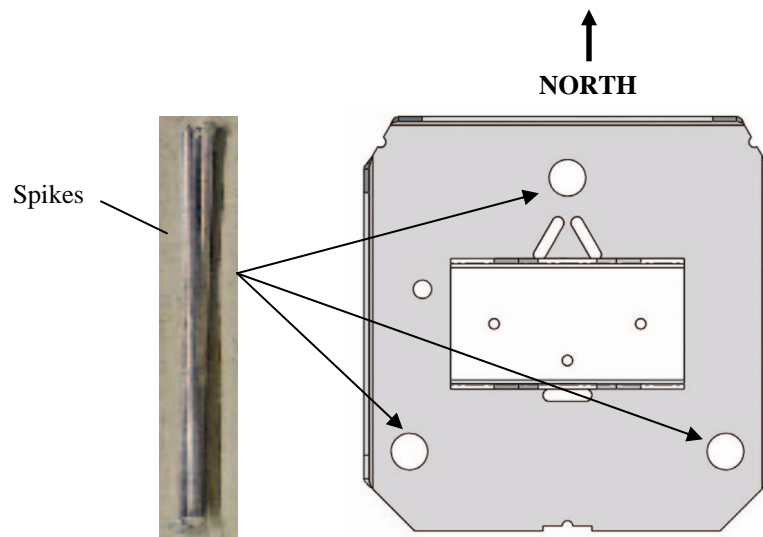


FIGURE 2.2-4. Spikes Installation

Step 4: Insert the Section 2 coupler into the top of Section 1 (see Figure 2.2-5).

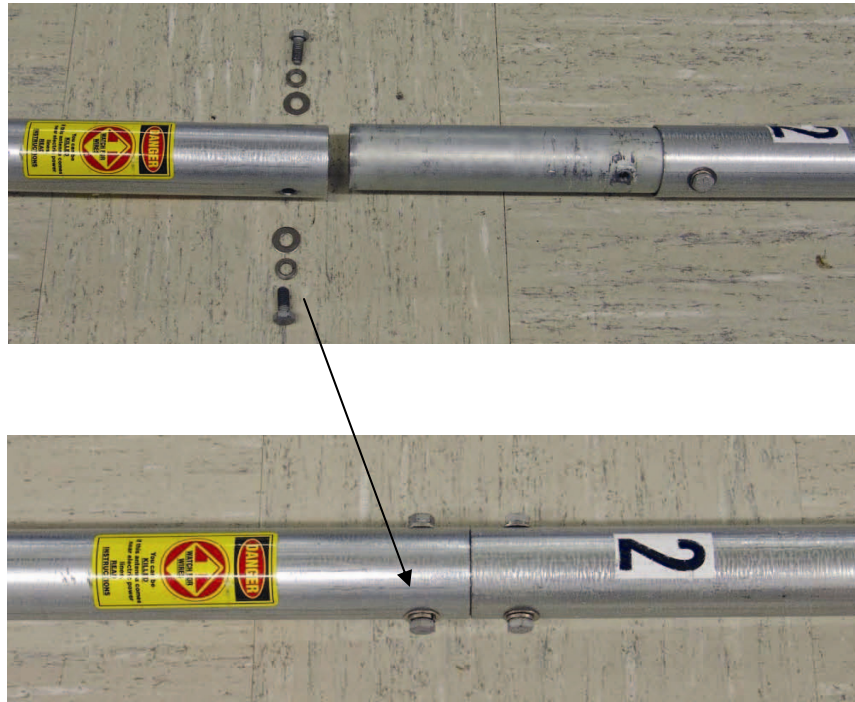


FIGURE 2.2-5. Coupler Installed in Top of Mast Section 1

Step 5: Secure joint with 2 flat washers, 2 lock washers and 2 bolts from the hardware bag (see Figure 2.2-6).



FIGURE 2.2-6. Bag Containing Hardware

Step 6: Assemble Section 3 to the top of Section 2 (see Figure 2.2-7).

NOTE The BLACK tape around Section 2 is a reference (11 foot level) for optional sensor mounts.



FIGURE 2.2-7. Mast Section 2 and Mast Section 3

Step 7: Remove the collars from Section 3 and place next to the mounting holes in Section 2 (see Figures 2.2-7 and 2.2-8).

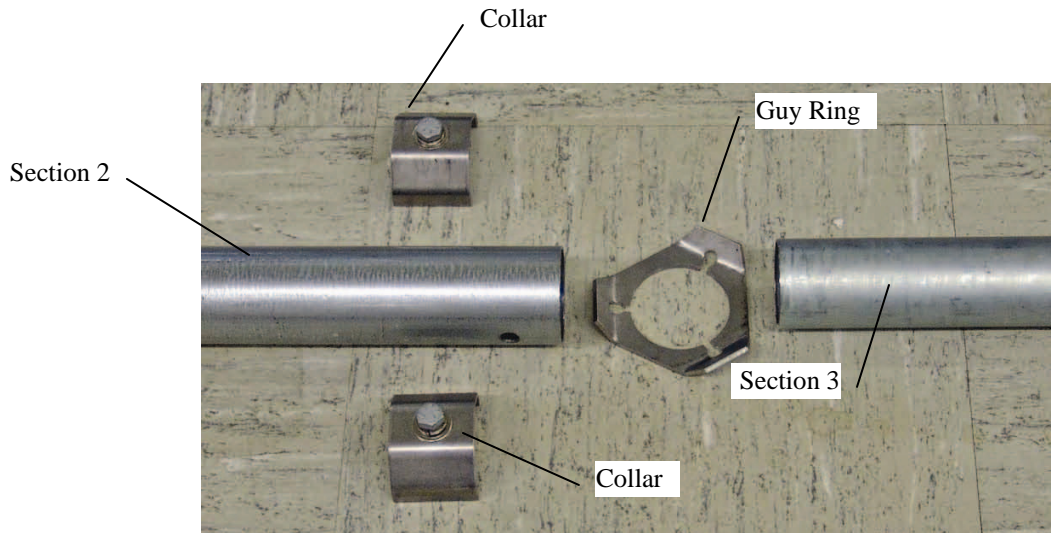


FIGURE 2.2-8. Guy Ring, Mast Section 2 and Mast Section 3

Step 8: Remove guy ring from bottom guy kit, PN 21663 (see Figures 2.2-8 and 2.2-9).



FIGURE 2.2-9. 21663 Bottom Guy Kit

Step 9: Place ball end of each guy cable into its slot in the guy ring and place guy ring into coupler of Section 3 (see Figure 2.2-10).

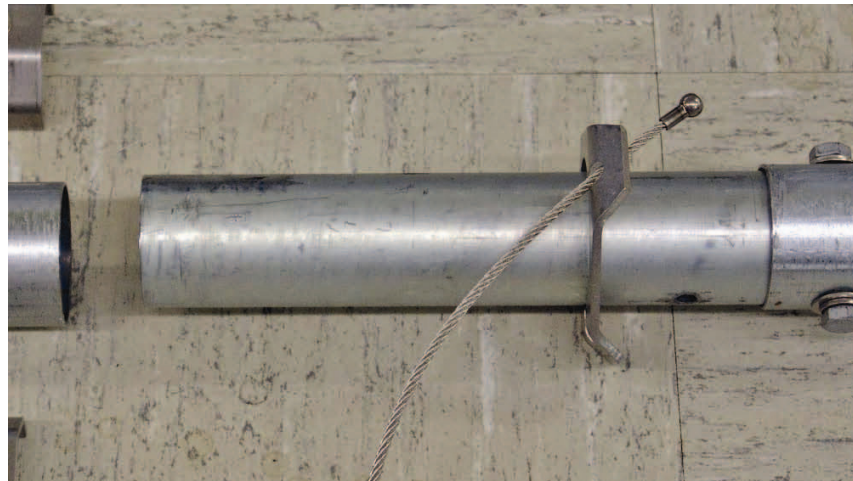


FIGURE 2.2-10. Guy Cable Inserted into Guy Ring

NOTE Only one of the three cable ends is shown.

Step 10: Slide coupler into Section 2 mast and assemble collars, as shown in Figure 2.2-11.

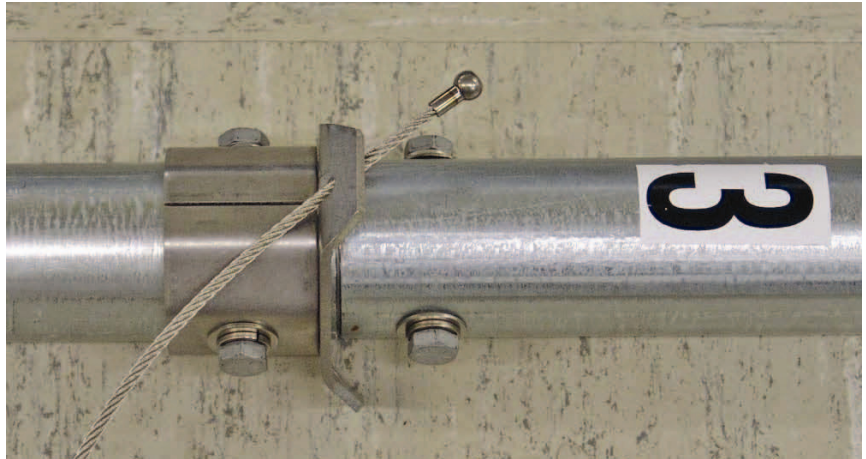


FIGURE 2.2-11. Mast Section 3 and Guy Ring/Collar Assembly

Step 11: Slide coupler end of Section 4 into the top of Section 3, and secure with remaining components from hardware bag (see Figure 2.2-12).

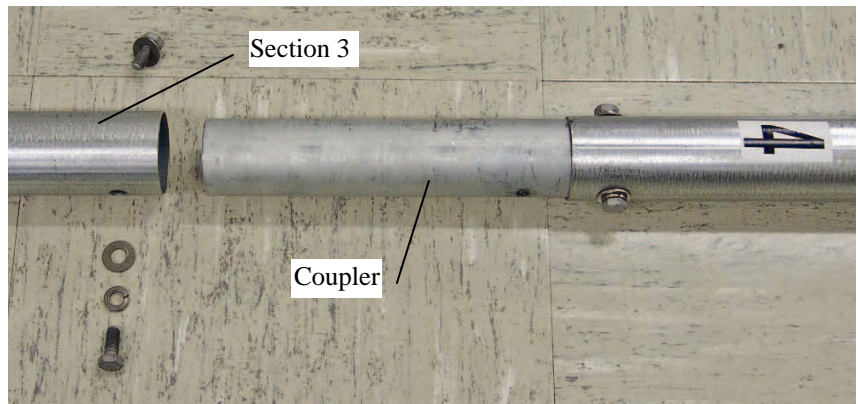


FIGURE 2.2-12. Mast Section 4 Ready to be Installed in Mast Section 3

Step 12: Remove collars from Section 5 (see Figure 2.2-13).

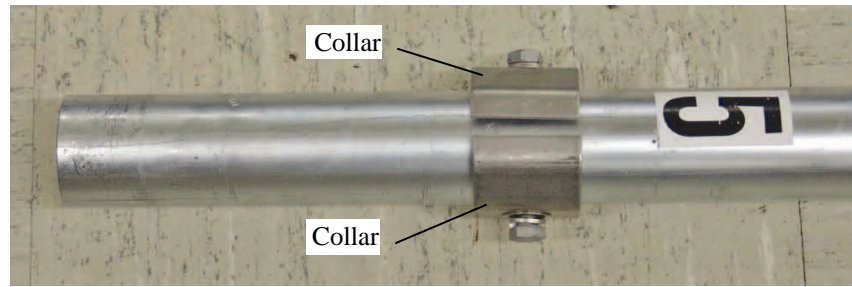


FIGURE 2.2-13. Mast Section 5

Step 13: Slide mast into Section 4 and assemble collars, as shown in Figure 2.2-14.

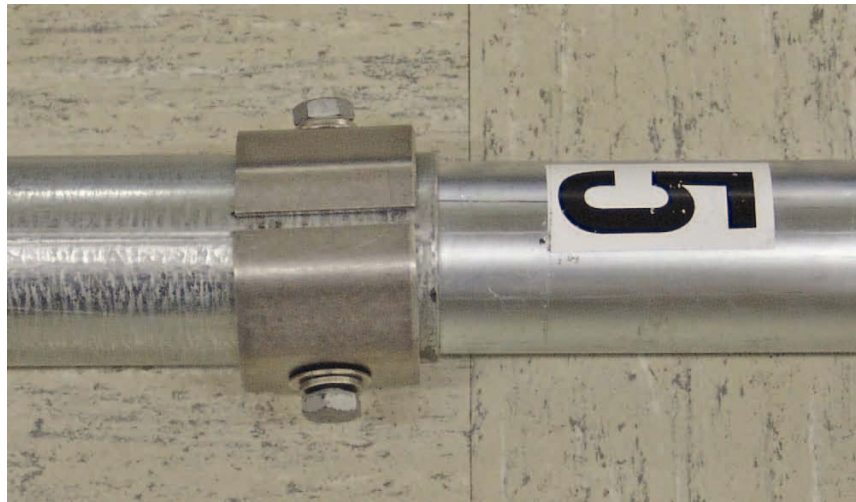


FIGURE 2.2-14. Mast Section 5 Installed in Mast Section 4

Step 14: Remove guy collar from 21661 guy kit (see Figure 2.2-15).



FIGURE 2.2-15. 21661 Guy Kit

Step 15: Place guy cable ball ends into guy ring and then slide ring down mast to collar (see Figure 2.2-16).

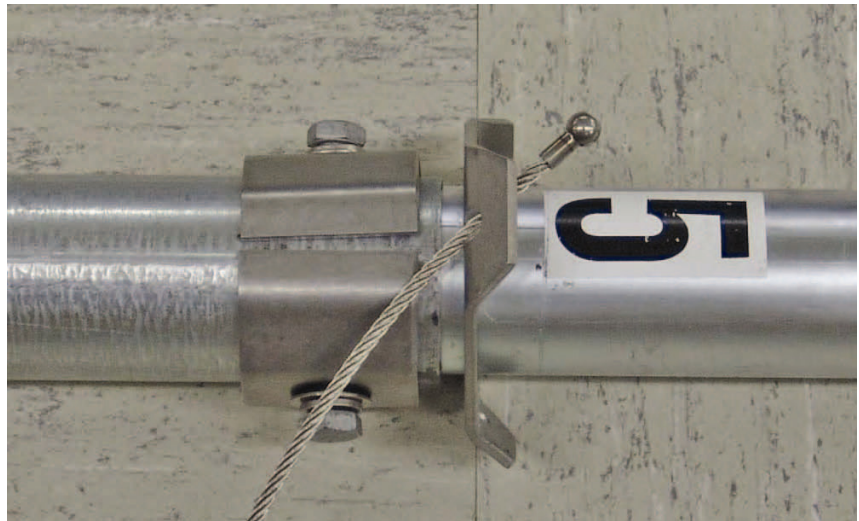


FIGURE 2.2-16. Mast Section 5 and Guy Ring/Collar Assembly

2.3 Lightning Rod Assembly and Mounting Instrumentation

Step 1: Fit lightning rod assembly (from PN 21660) to top of Section 5 mast (see Figure 2.3-1).



FIGURE 2.3-1. Lightning Rod Assembly

Step 2: Place clamp onto top of mast Section 5 and tighten (see Figure 2.3-2).

Step 3: Insert rod into clamp and tighten (see Figure 2.3-2).

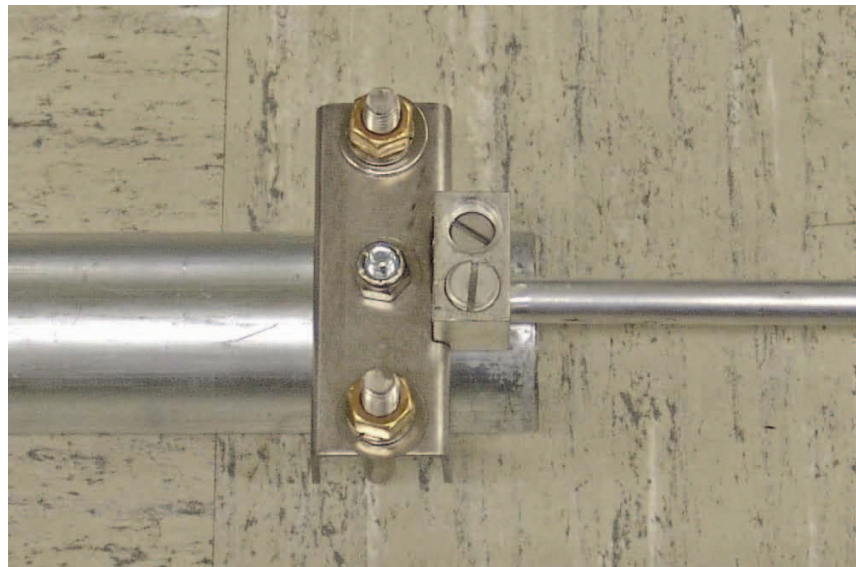


FIGURE 2.3-2. Installed Lightning Rod

Step 4: Assemble enclosures, sensors and tie cables to mast, as required.

2.4 Anchor Installation



FIGURE 2.4-1. Tape Measure in Slot for South Anchor

Step 1: For the South anchor, place tape measure into slot in base centering tape within notch on edge of base. Measure to 20 ft (see Figure 2.4-1).

Step 2: At 20 ft, install the duckbill anchor with drive rod (see Figure 2.4-2). The anchor needs to be driven into the ground at a 45° angle (see Figure 2.4-3). Drive anchor until the loop or metal ring is several inches above the ground.

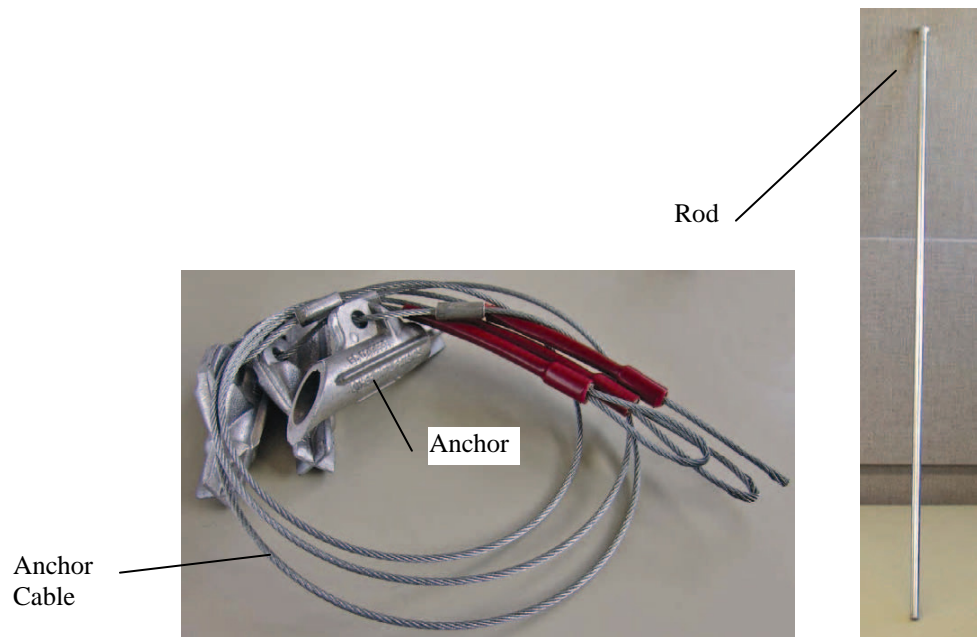


FIGURE 2.4-2. 19282 Duckbill Anchor and Cable Assembly (left).
The 25699 has a threaded rod instead of the cable.
The drive rod (right) is used for both the 19282 and 25699.

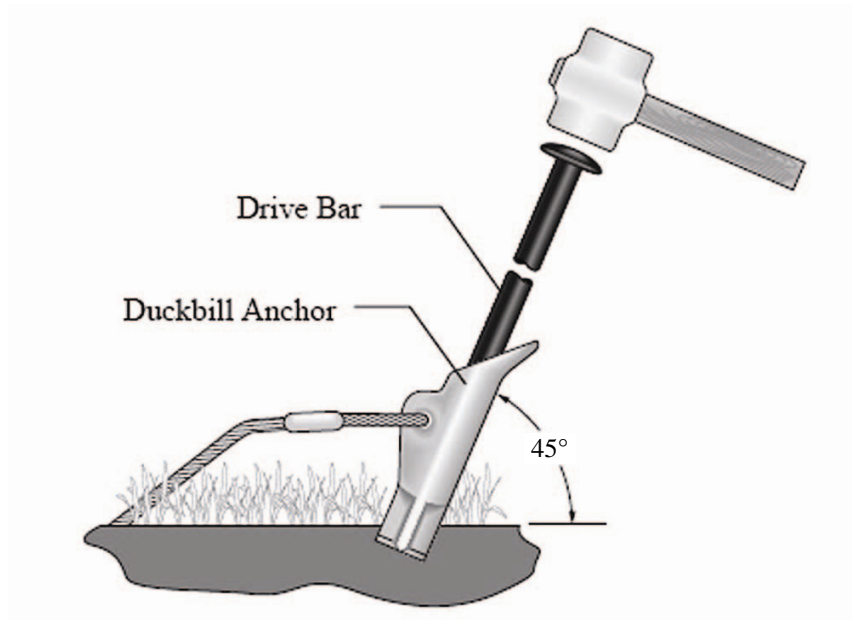


FIGURE 2.4-3. Anchor Driven into Ground at 45° Angle

Step 3: With a rod through the loop or metal ring, pull up on the cable or threaded rod until the anchor rotates and locks (see Figure 2.4-4).

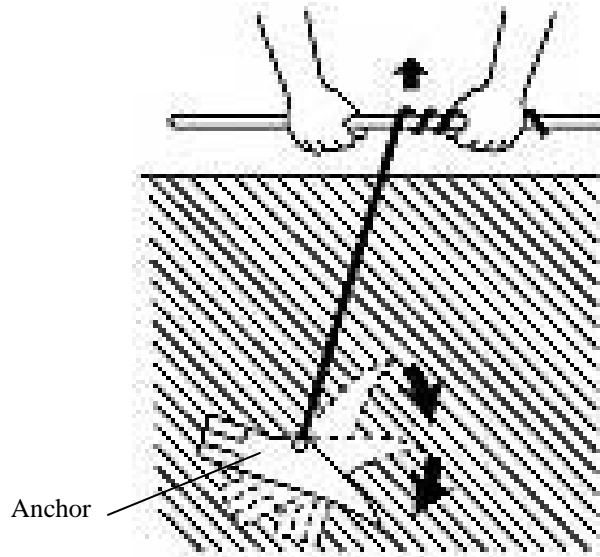


FIGURE 2.4-4. Locking Anchor

Step 4: Fill-in the hole around the cable or threaded rod with loose dirt and tamp firm.

Step 5: Repeat process for the NE (Figure 2.4-5) and NW anchors.

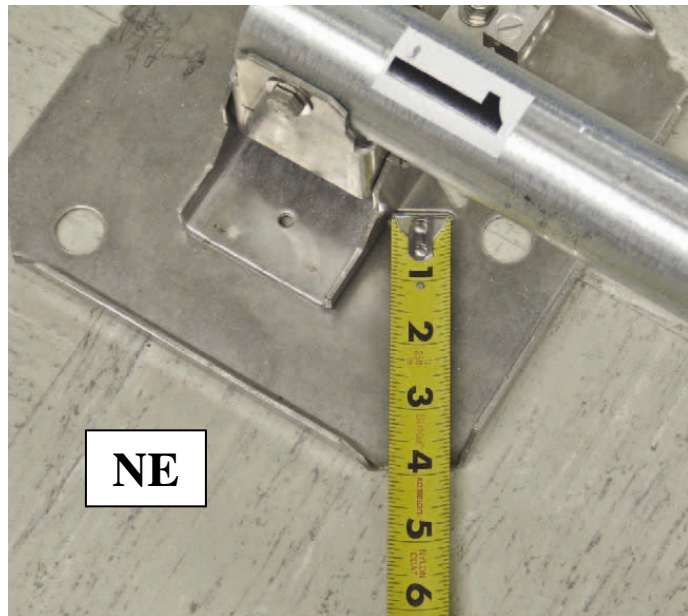


FIGURE 2.4-5. Tape Measure in Slot for North East Anchor

Step 6: Attach guy wires to anchors by first opening the turnbuckle to the widest setting. Attach turnbuckle to wedge end of the guy cable, and then attach the other end of the turnbuckle to an anchor (see Figure 2.4-6).

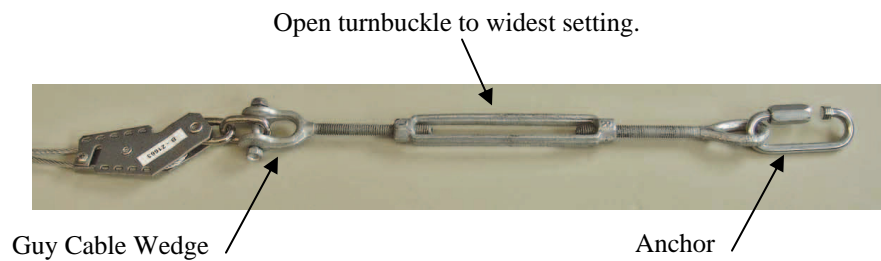


FIGURE 2.4-6. Turnbuckle Fastened to Guy Cable and Anchor

Step 7: If using rope ratchet to assist assembly, set to 7 feet and attach to tension clamp on cable and to anchor end. Do this for both NE and NW anchors and top and bottom guy cables (see Figures 2.4-7 and 2.4-8).

NOTE

Do not connect the SOUTH cables at this time.

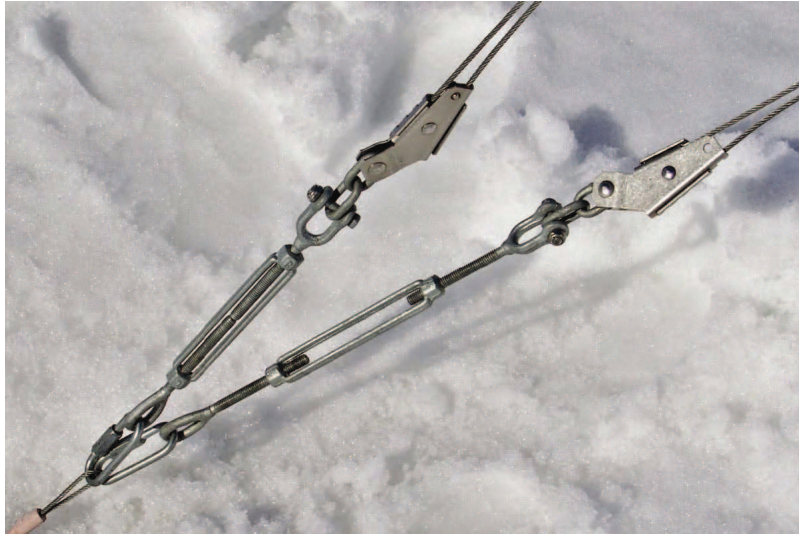


FIGURE 2.4-7. Top and Bottom Guy Cables Fastened to an Anchor



FIGURE 2.4-8. Rope Ratchet Assists Assembly

Step 8: Course adjustments to cable length are made by loosening screw clamp and then releasing wedge with a blade screwdriver (see Figure 2.4-9). This allows the cable to be adjusted through the wedge clamp.

NOTE Retighten screw when adjustment is complete.



FIGURE 2.4-9. Adjusting Cable through Wedge Clamp

2.5 Raise, Plumb Mast and Final Cable Tensioning

Step 1: With NW and NE cables attached to anchors have one person lift mast, while another person pulls on the SOUTH cables to bring mast to an upright position (see Figure 2.5-1). If using rope ratchets, adjust them to allow further steps.



FIGURE 2.5-1. Raising the Mast

Step 2: Attach SOUTH cables to anchor. While first person holds mast and uses a pole level, the second person adjusts each of the bottom guy cable wedge clamps, maintaining level in all directions (see Figure 2.5-2). The rope ratchet can be used to temporarily remove the load from the wedge assembly during wedge adjustments.



FIGURE 2.5-2. Pole Level Ensures Vertical Mast

Step 3: Repeat process with the top guy cables to establish a straight mast.

Step 4: Apply further tensioning using the turnbuckles (see Figure 2.5-3).



FIGURE 2.5-3. Adjusting Turnbuckles

Step 5: Adjust each cable turnbuckle to maintain plumb and increase cable tension. A deflection of 3 inches when using a 4.4 pound (2N) perpendicular force, 68 inches from the duckbill anchor loop equates to 100 pounds of tension in the cables (see Figure 2.5-4).

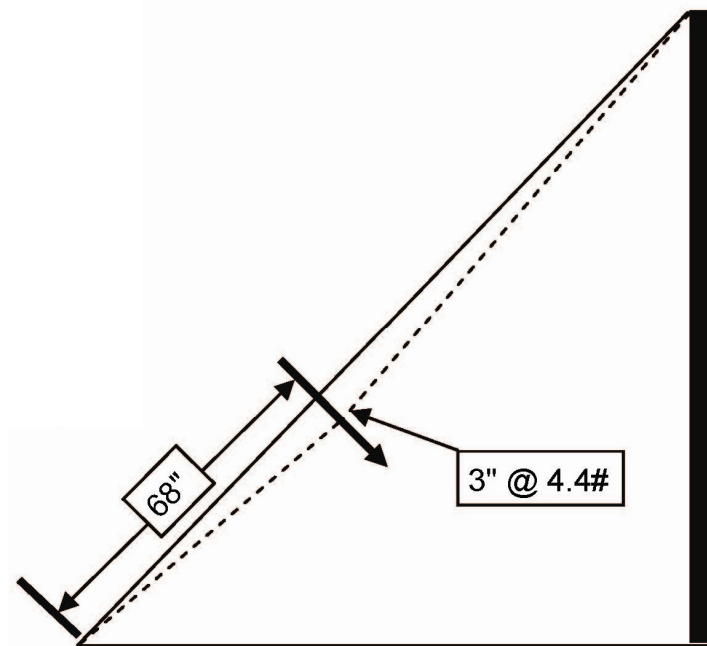


FIGURE 2.5-4. Guy Cables with 100 lbs of Tension

Step 6: After tensioning the top guy cables, recheck the bottom guy cables.

Adjust, as necessary.

3. Maintenance

Check and adjust guy cable tension at least once a month, and after wind gusts exceeding 50 mph.

Campbell Scientific Companies

Campbell Scientific, Inc. (CSI)

815 West 1800 North
Logan, Utah 84321
UNITED STATES

www.campbellsci.com • info@campbellsci.com

Campbell Scientific Africa Pty. Ltd. (CSAf)

PO Box 2450
Somerset West 7129
SOUTH AFRICA

www.csafrica.co.za • cleroux@csafrica.co.za

Campbell Scientific Australia Pty. Ltd. (CSA)

PO Box 444
Thuringowa Central
QLD 4812 AUSTRALIA

www.campbellsci.com.au • info@campbellsci.com.au

Campbell Scientific do Brazil Ltda. (CSB)

Rua Luisa Crapsi Orsi, 15 Butantã
CEP: 005543-000 São Paulo SP BRAZIL

www.campbellsci.com.br • suporte@campbellsci.com.br

Campbell Scientific Canada Corp. (CSC)

11564 - 149th Street NW
Edmonton, Alberta T5M 1W7
CANADA

www.campbellsci.ca • dataloggers@campbellsci.ca

Campbell Scientific Centro Caribe S.A. (CSCC)

300 N Cementerio, Edificio Breller
Santo Domingo, Heredia 40305
COSTA RICA

www.campbellsci.cc • info@campbellsci.cc

Campbell Scientific Ltd. (CSL)

Campbell Park
80 Hathern Road
Shepshed, Loughborough LE12 9GX
UNITED KINGDOM

www.campbellsci.co.uk • sales@campbellsci.co.uk

Campbell Scientific Ltd. (France)

Miniparc du Verger - Bat. H
1, rue de Terre Neuve - Les Ulis
91967 COURTABOEUF CEDEX
FRANCE

www.campbellsci.fr • info@campbellsci.fr

Campbell Scientific Spain, S. L.

Avda. Pompeu Fabra 7-9, local 1
08024 Barcelona
SPAIN

www.campbellsci.es • info@campbellsci.es

Please visit www.campbellsci.com to obtain contact information for your local US or International representative.