

INSTRUCTION MANUAL



SP65 Solar Panel

Revision: 7/08



Copyright © 1987 - 2008
Campbell Scientific, Inc.

Warranty and Assistance

The **SP65 SOLAR PANEL** is warranted by CAMPBELL SCIENTIFIC, INC. to be free from defects in materials and workmanship under normal use and service for twelve (12) months from date of shipment unless specified otherwise. Batteries have no warranty. CAMPBELL SCIENTIFIC, INC.'s obligation under this warranty is limited to repairing or replacing (at CAMPBELL SCIENTIFIC, INC.'s option) defective products. The customer shall assume all costs of removing, reinstalling, and shipping defective products to CAMPBELL SCIENTIFIC, INC. CAMPBELL SCIENTIFIC, INC. will return such products by surface carrier prepaid. This warranty shall not apply to any CAMPBELL SCIENTIFIC, INC. products which have been subjected to modification, misuse, neglect, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied, including warranties of merchantability or fitness for a particular purpose. CAMPBELL SCIENTIFIC, INC. is not liable for special, indirect, incidental, or consequential damages.

Products may not be returned without prior authorization. The following contact information is for US and International customers residing in countries served by Campbell Scientific, Inc. directly. Affiliate companies handle repairs for customers within their territories. Please visit www.campbellsci.com to determine which Campbell Scientific company serves your country. To obtain a Returned Materials Authorization (RMA), contact CAMPBELL SCIENTIFIC, INC., phone (435) 753-2342. After an applications engineer determines the nature of the problem, an RMA number will be issued. Please write this number clearly on the outside of the shipping container. CAMPBELL SCIENTIFIC's shipping address is:

CAMPBELL SCIENTIFIC, INC.

RMA#_____

815 West 1800 North

Logan, Utah 84321-1784

CAMPBELL SCIENTIFIC, INC. does not accept collect calls.

SP65 Table of Contents

PDF viewers note: These page numbers refer to the printed version of this document. Use the Adobe Acrobat® bookmarks tab for links to specific sections.

1. General	1
2. Specifications	1
3. Installation.....	1
3.1 Mounting	1
3.2 Orientation	2
3.3 Installation of Morningstar SunSaver SS-10-12V Regulator	4
4. Maintenance	5
5. Power Considerations.....	5
5.1 Solar Power and Lead Acid Batteries	5
5.2 Voltage Regulator.....	6

Appendix

A. Assembly Instructions for 65 Watt Solar Panel with Mounting Bracket	A-1
---	------------

Figures

1. Solar Panel Mounting	2
2. Angle Settings on Mounting Bracket	3
3. Morningstar's SunSaver SS-10-12V regulator mounted on an enclosure backplate.....	5
4. Solar Panel Orientation.....	6
A-1. 65 Watt Solar Panel Assembly Instructions	A-1

Tables

1. Solar Panel Tilt Angle	3
2. Configurations for Desired Angles.....	3
A-1. Mounting Bracket Parts List.....	A-2

SP65 Solar Panel

1. General

Solar panels are a photovoltaic power source used for charging lead acid batteries. The SP65 has two leads terminated with spade lugs that connect to the regulator that is shipped with the SP65. The 15' cable shipped with the SP65 connects the regulator to the battery. Do not use the SP65 with the PS100 or CH100.

2. Specifications

	SP65*
Typical peak power (Pp)	65 W
Voltage @ peak power (Vpp) (voltage from solar panel before regulator)	17.6 V
Current @ peak power (Ipp)	3.69 A
Guaranteed minimum peak power	60 W
Temperature coefficient of power	-(0.5 ± 0.05)%/°C
Length, cm	111.1
Width, cm	50.2
Depth, cm	5
Weight, kg	7.2

NOTE

The above solar panel characteristics assume a 1 kilowatt per square meter illumination and a solar panel temperature of 25°C. Individual panels may vary up to 10%. The output panel voltage increases as the panel temperature decreases.

*An SP65 can be connected to another SP65 to provide 130 W of typical peak power.

Regulator

Model: Morningstar SunSaver SS-10-12V
Temperature Compensation (mV/°C): -28
Self Consumption: 6 to 10 mA
Operating Temperature: -40° to +85°C

3. Installation

3.1 Mounting

The panel should be mounted facing south if located in the Northern Hemisphere, or facing north in the Southern Hemisphere. The solar panel mounts to the mast or leg of a tripod, or any 1 5/8" schedule 40 pipe, see Figure 1. The panel should be mounted to the pipe using the U-bolts and 5/16

NC (course) nuts provided with the solar panel. The nuts fastening the bracket to the pipe should be as tight as possible without bending the bracket.

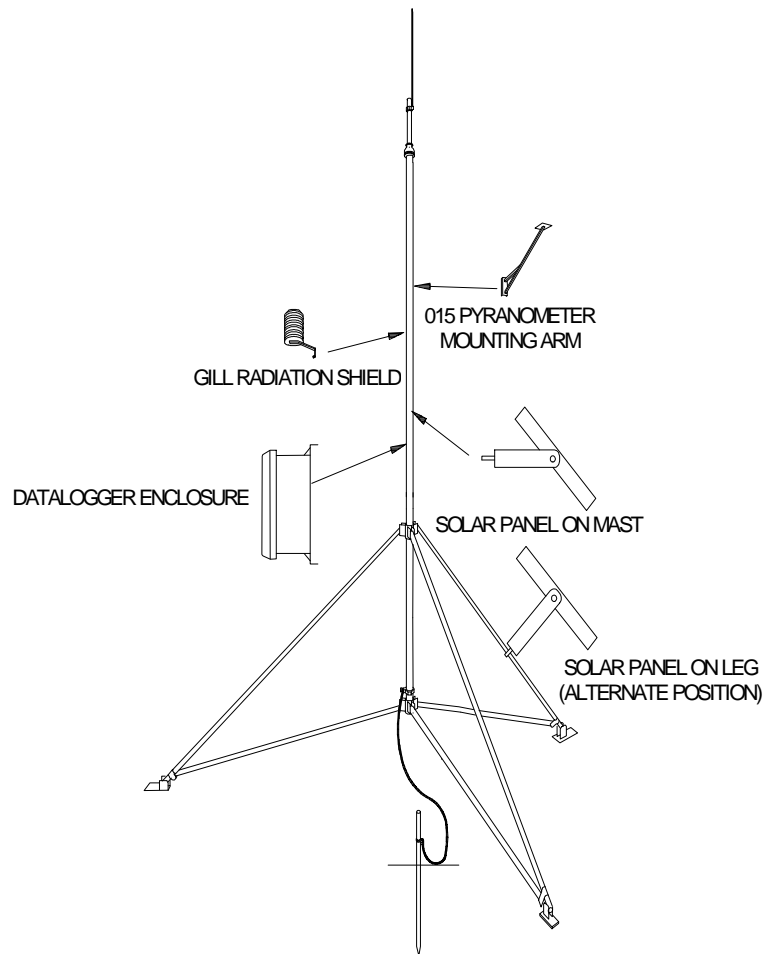


FIGURE 1. Solar Panel Mounting

3.2 Orientation


The solar panel should be oriented to receive maximum insolation (incident solar radiation) over the course of a year. Suggested tilt angles of the solar panel are given in Table 1.

After determining the tilt angle, loosen the 5/16" nuts on each side of the solar panel, adjust the panel, and tighten the two nuts to secure the position. See Figure 2.

TABLE 1. Solar Panel Tilt Angle*

<u>Site Latitude (N or S)</u>	<u>Tilt Angle</u>
0 – 10°	10°
11 – 20°	Latitude +5°
21 – 45	Latitude +10°
46 – 65	Latitude +15°
> 65	80°

* From "Design Aids for Small PV Power Systems", Solorex Corp.

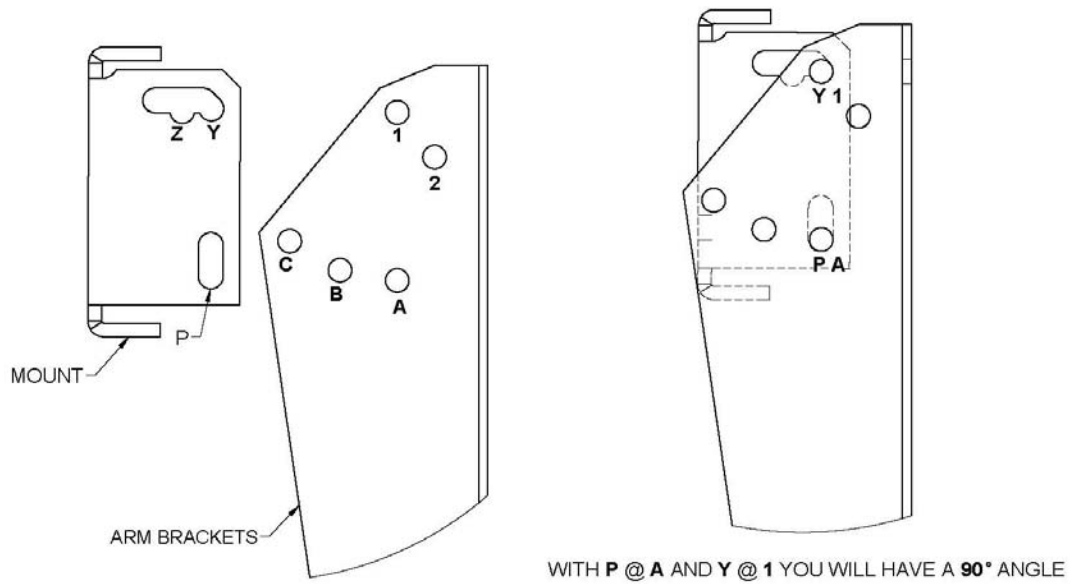**FIGURE 2. Angle Settings on Mounting Bracket****TABLE 2. Configurations for Desired Angles**

Hole Locations	Angle
Holes P and A Aligned with Holes 1 and Y	90
Holes P and A Aligned with Holes 1 and Z	80
Holes P and B Aligned with Holes 1 and Y	70
Holes P and B Aligned with Holes 1 and Z	60
Holes P and C Aligned with Holes 1 and Y	50
Holes P and C Aligned with Holes 1 and Z	40
Holes P and C Aligned with Holes 2 and Y	30
Holes P and C Aligned with Holes 2 and Z	20

3.3 Installation of Morningstar SunSaver SS-10-12V Regulator

NOTE

For safety reasons, completely cover the solar panel to limit output current and voltage. If nothing is available to cover the panel, be careful not to short solar panel (+) and (-) leads together.

1. Using the supplied mounting hardware, install the Morningstar SunSaver SS-10-12V regulator to the mounting plate of an environmental enclosure (see Figure 3).
2. Using the supplied red and black power cables, secure the black wire to terminal lug #1 marked battery (-) on the regulator. Connect the pigtailed end of the cable to the negative battery terminal. Secure the red wire to terminal lug #2 marked battery (+) on the regulator. Connect the pigtailed end of the cable to the battery's positive terminal. With the battery connected and no solar panel input, the green charging LED **SHOULD NOT** be on.
3. Connect the black (-) wire from the SP65 power cable to terminal lug #3 marked solar (-) on the regulator. Connect the red (+) wire from the SP65 power cable to terminal lug #4 marked solar (+) on the SunSaver regulator. If using a sealed rechargeable battery such as our BP24, then verify that the metal jumper is installed to configure the regulator to recharge sealed rechargeable batteries (see Figure 3). If using a flooded battery (e.g., car or marine deep cycle), then remove the jumper. Also note that no connections are made on the load terminals of the regulator for this application (see Figure 3).
4. If charge current is available from the solar panel, the green charge LED **WILL LIGHT UP**. This will verify proper operation and wiring of the regulator.



FIGURE 3. Morningstar's SunSaver SS-10-12V regulator mounted on an enclosure backplate.

4. Maintenance

An occasional cleaning of the glass improves the solar panel's efficiency.

If a problem with the solar panel is suspected, the panel may be checked by measuring the voltage output. Check the voltage with a voltmeter connected between the two leads of the solar panel. There must be solar radiation incident on the panel and there must be a load connected to the solar panel. The load can be the datalogger, other equipment, or a 75 ohm resistor capable of dissipating solar panel power between the two leads. No voltage output implies a bad solar panel, regulator, or cable. The magnitude of the voltage output depends on the incident solar radiation.

5. Power Considerations

5.1 Solar Power and Lead Acid Batteries

The solar panel converts light energy to electricity, or specifically direct current. The direct current produced is used as a charging source for lead acid batteries.

The solar panel operates in both direct and diffuse light (cloudy days), but not at night.

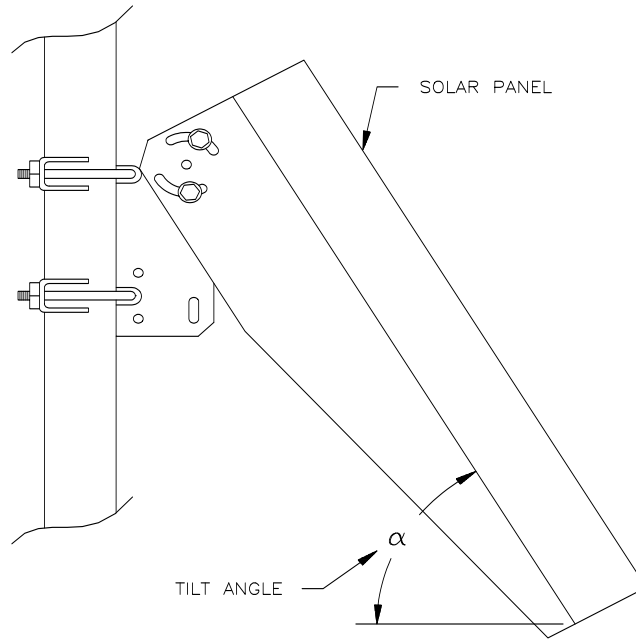


FIGURE 4. Solar Panel Orientation

The minimum battery size and solar panel output required depends on 1) the average current drain of the system, 2) the maximum time the battery must supply power to the system without being charged, and 3) the location of the site. When some batteries are discharged below a specified voltage, the battery becomes damaged and cannot be recharged.

The battery supplies power directly to the operating system, the solar panel supplies power to recharge the battery. Therefore, on the average, the solar panel must provide at least as much power to the battery as is being used by the system.

The battery must have enough capacity to power the system during times of no charging (night) or low charging (stormy winter days).

5.2 Voltage Regulator

The regulator has two basic functions: 1) blocks any current flow from the battery to the solar panel, and 2) limits the source current to the battery.

The SP65 is shipped with Morningstar's SunSaver SS-10-12V regulator. The regulator connects to the battery via the 15' cable shipped with the SP65. The regulator and battery should be housed in an environmental enclosure. Mounting brackets are included with the regulator for attachment to an enclosure backplate.

Appendix A. Assembly Instructions for 65 Watt Solar Panel with Mounting Bracket

1. ATTACH #2 AND #3 TO PANEL(#1) AS SHOWN USING #10,6,8 AND 7 IN (2) PLCS.
2. ATTACH #4 TO #2 AND #3 IN HOLES FOR DESIRED ANGLE USING #10, 6 (2), 8 AND 7 IN (4) PLCS.
3. WITH BRACKETS FASTENED TOGETHER YOU MAY NOW ATTACH TO STRUCTURE.
4. IF YOU ARE MOUNTING TO A TOWER STRUCTURE, THE (4) #9 U-BOLTS WITH #5 SPACERS ARE TO BE USED.
5. IF YOU ARE MOUNTING TO A MAST OR SINGLE POLE, (2) #11 ARE TO BE USED WITH #6,7 AND 8.

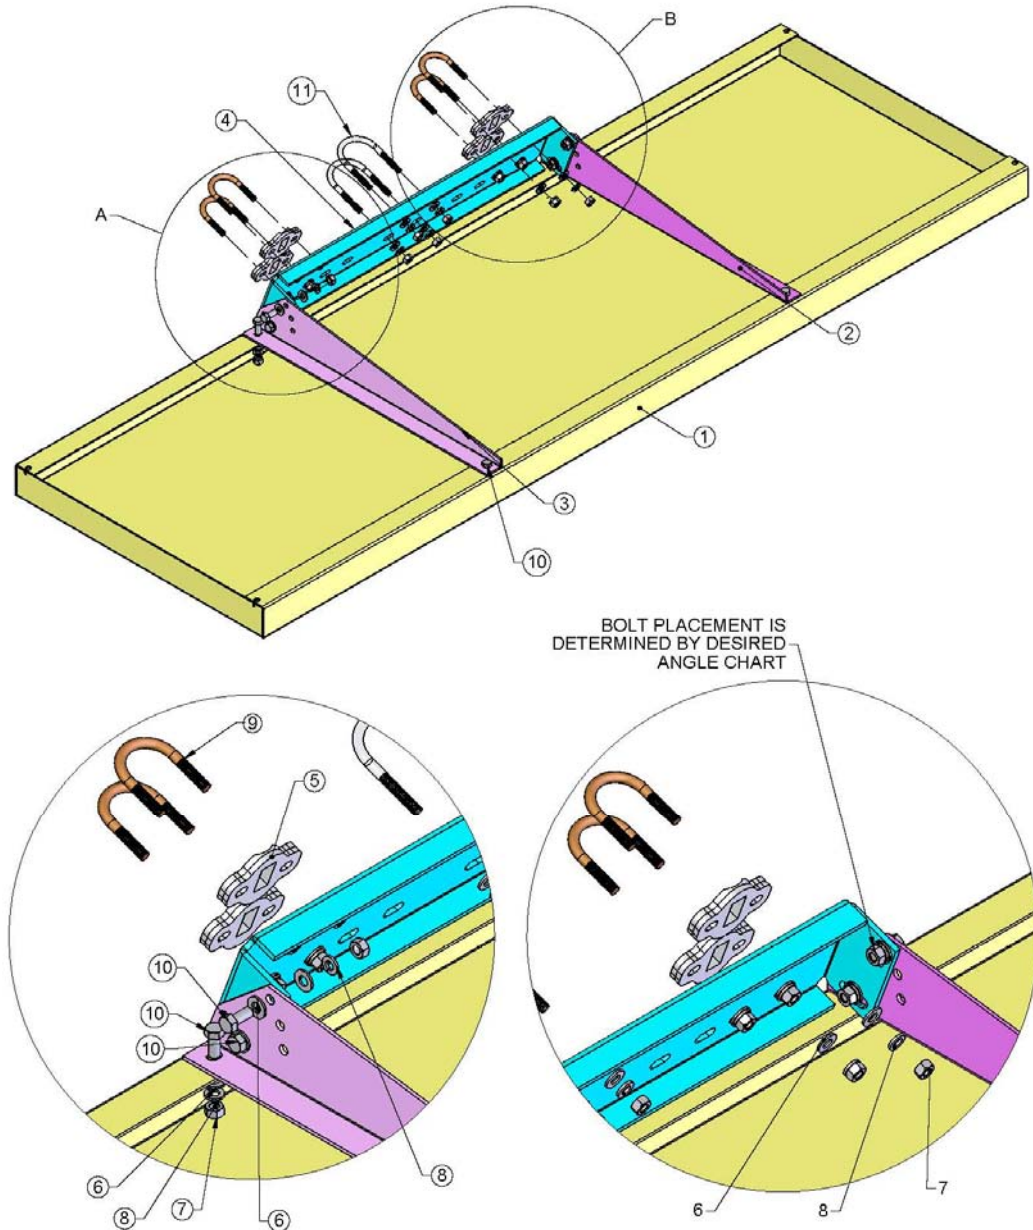


FIGURE A-1. 65 Watt Solar Panel Assembly Instructions

TABLE A-1. Mounting Bracket Parts List		
Item #	Description	Qty
1	65 W Solar Panel	1
2	Right Arm Bracket	1
3	Left Arm Bracket	1
4	Mount	1
5	Spacer	4
6	Flat Washer	24
7	5/16-18 Nut	8
8	Lock Washer	20
9	5/16-18 x 1.50 U-Bolt w/nuts	4
10	5/16-18 x .750 Hex Bolt	8
11	5/16-18 x 2.0 U-Bolt w/nuts	2

Campbell Scientific Companies

Campbell Scientific, Inc. (CSI)

815 West 1800 North
Logan, Utah 84321
UNITED STATES
www.campbellsci.com
info@campbellsci.com

Campbell Scientific Africa Pty. Ltd. (CSAf)

PO Box 2450
Somerset West 7129
SOUTH AFRICA
www.csafrica.co.za
cleroux@csafrica.co.za

Campbell Scientific Australia Pty. Ltd. (CSA)

PO Box 444
Thuringowa Central
QLD 4812 AUSTRALIA
www.campbellsci.com.au
info@campbellsci.com.au

Campbell Scientific do Brazil Ltda. (CSB)

Rua Luisa Crapsi Orsi, 15 Butantã
CEP: 005543-000 São Paulo SP BRAZIL
www.campbellsci.com.br
suporte@campbellsci.com.br

Campbell Scientific Canada Corp. (CSC)

11564 - 149th Street NW
Edmonton, Alberta T5M 1W7
CANADA
www.campbellsci.ca
dataloggers@campbellsci.ca

Campbell Scientific Ltd. (CSL)

Campbell Park
80 Hathern Road
Shepshed, Loughborough LE12 9GX
UNITED KINGDOM
www.campbellsci.co.uk
sales@campbellsci.co.uk

Campbell Scientific Ltd. (France)

Miniparc du Verger - Bat. H
1, rue de Terre Neuve - Les Ulis
91967 COURTABOEUF CEDEX
FRANCE
www.campbellsci.fr
info@campbellsci.fr

Campbell Scientific Spain, S. L.

Psg. Font 14, local 8
08013 Barcelona
SPAIN
www.campbellsci.es
info@campbellsci.es