


# INSTRUCTION MANUAL



## CS451/CS456 Submersible Pressure Transducer

Revision: 7/14

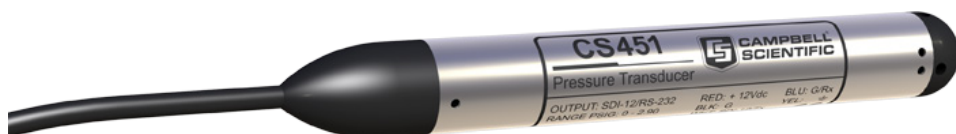

Copyright © 2009 - 2014  
Campbell Scientific, Inc.



# ***Limited Warranty***

---

“Products manufactured by CSI are warranted by CSI to be free from defects in materials and workmanship under normal use and service for twelve months from the date of shipment unless otherwise specified in the corresponding product manual. (Product manuals are available for review online at [www.campbellsci.com](http://www.campbellsci.com).) Products not manufactured by CSI, but that are resold by CSI, are warranted only to the limits extended by the original manufacturer. Batteries, fine-wire thermocouples, desiccant, and other consumables have no warranty. CSI’s obligation under this warranty is limited to repairing or replacing (at CSI’s option) defective Products, which shall be the sole and exclusive remedy under this warranty. The Customer assumes all costs of removing, reinstalling, and shipping defective Products to CSI. CSI will return such Products by surface carrier prepaid within the continental United States of America. To all other locations, CSI will return such Products best way CIP (port of entry) per Incoterms ® 2010. This warranty shall not apply to any Products which have been subjected to modification, misuse, neglect, improper service, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied. The warranty for installation services performed by CSI such as programming to customer specifications, electrical connections to Products manufactured by CSI, and Product specific training, is part of CSI’s product warranty. **CSI EXPRESSLY DISCLAIMS AND EXCLUDES ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.** CSI hereby disclaims, to the fullest extent allowed by applicable law, any and all warranties and conditions with respect to the Products, whether express, implied or statutory, other than those expressly provided herein.”

# Assistance

---

Products may not be returned without prior authorization. The following contact information is for US and international customers residing in countries served by Campbell Scientific, Inc. directly. Affiliate companies handle repairs for customers within their territories. Please visit [www.campbellsci.com](http://www.campbellsci.com) to determine which Campbell Scientific company serves your country.

To obtain a Returned Materials Authorization (RMA), contact CAMPBELL SCIENTIFIC, INC., phone (435) 227-9000. After an applications engineer determines the nature of the problem, an RMA number will be issued. Please write this number clearly on the outside of the shipping container. Campbell Scientific's shipping address is:

**CAMPBELL SCIENTIFIC, INC.**

RMA# \_\_\_\_\_  
815 West 1800 North  
Logan, Utah 84321-1784

For all returns, the customer must fill out a "Statement of Product Cleanliness and Decontamination" form and comply with the requirements specified in it. The form is available from our web site at [www.campbellsci.com/repair](http://www.campbellsci.com/repair). A completed form must be either emailed to [repair@campbellsci.com](mailto:repair@campbellsci.com) or faxed to (435) 227-9106. Campbell Scientific is unable to process any returns until we receive this form. If the form is not received within three days of product receipt or is incomplete, the product will be returned to the customer at the customer's expense. Campbell Scientific reserves the right to refuse service on products that were exposed to contaminants that may cause health or safety concerns for our employees.

# Precautions

---

**DANGER — MANY HAZARDS ARE ASSOCIATED WITH INSTALLING, USING, MAINTAINING, AND WORKING ON OR AROUND TRIPODS, TOWERS, AND ANY ATTACHMENTS TO TRIPODS AND TOWERS SUCH AS SENSORS, CROSSARMS, ENCLOSURES, ANTENNAS, ETC.** FAILURE TO PROPERLY AND COMPLETELY ASSEMBLE, INSTALL, OPERATE, USE, AND MAINTAIN TRIPODS, TOWERS, AND ATTACHMENTS, AND FAILURE TO HEED WARNINGS, INCREASES THE RISK OF DEATH, ACCIDENT, SERIOUS INJURY, PROPERTY DAMAGE, AND PRODUCT FAILURE. TAKE ALL REASONABLE PRECAUTIONS TO AVOID THESE HAZARDS. CHECK WITH YOUR ORGANIZATION'S SAFETY COORDINATOR (OR POLICY) FOR PROCEDURES AND REQUIRED PROTECTIVE EQUIPMENT PRIOR TO PERFORMING ANY WORK.

Use tripods, towers, and attachments to tripods and towers only for purposes for which they are designed. Do not exceed design limits. Be familiar and comply with all instructions provided in product manuals. Manuals are available at [www.campbellsci.com](http://www.campbellsci.com) or by telephoning 435-227-9000 (USA). You are responsible for conformance with governing codes and regulations, including safety regulations, and the integrity and location of structures or land to which towers, tripods, and any attachments are attached. Installation sites should be evaluated and approved by a qualified engineer. If questions or concerns arise regarding installation, use, or maintenance of tripods, towers, attachments, or electrical connections, consult with a licensed and qualified engineer or electrician.

## General

- Prior to performing site or installation work, obtain required approvals and permits. Comply with all governing structure-height regulations, such as those of the FAA in the USA.
- Use only qualified personnel for installation, use, and maintenance of tripods and towers, and any attachments to tripods and towers. The use of licensed and qualified contractors is highly recommended.
- Read all applicable instructions carefully and understand procedures thoroughly before beginning work.
- Wear a **hardhat** and **eye protection**, and take **other appropriate safety precautions** while working on or around tripods and towers.
- **Do not climb** tripods or towers at any time, and prohibit climbing by other persons. Take reasonable precautions to secure tripod and tower sites from trespassers.
- Use only manufacturer recommended parts, materials, and tools.

## Utility and Electrical

- **You can be killed** or sustain serious bodily injury if the tripod, tower, or attachments you are installing, constructing, using, or maintaining, or a tool, stake, or anchor, come in **contact with overhead or underground utility lines**.
- Maintain a distance of at least one-and-one-half times structure height, or 20 feet, or the distance required by applicable law, **whichever is greater**, between overhead utility lines and the structure (tripod, tower, attachments, or tools).
- Prior to performing site or installation work, inform all utility companies and have all underground utilities marked.
- Comply with all electrical codes. Electrical equipment and related grounding devices should be installed by a licensed and qualified electrician.

## Elevated Work and Weather

- Exercise extreme caution when performing elevated work.
- Use appropriate equipment and safety practices.
- During installation and maintenance, keep tower and tripod sites clear of un-trained or non-essential personnel. Take precautions to prevent elevated tools and objects from dropping.
- Do not perform any work in inclement weather, including wind, rain, snow, lightning, etc.

## Maintenance

- Periodically (at least yearly) check for wear and damage, including corrosion, stress cracks, frayed cables, loose cable clamps, cable tightness, etc. and take necessary corrective actions.
- Periodically (at least yearly) check electrical ground connections.

WHILE EVERY ATTEMPT IS MADE TO EMBODY THE HIGHEST DEGREE OF SAFETY IN ALL CAMPBELL SCIENTIFIC PRODUCTS, THE CUSTOMER ASSUMES ALL RISK FROM ANY INJURY RESULTING FROM IMPROPER INSTALLATION, USE, OR MAINTENANCE OF TRIPODS, TOWERS, OR ATTACHMENTS TO TRIPODS AND TOWERS SUCH AS SENSORS, CROSSARMS, ENCLOSURES, ANTENNAS, ETC.



# Table of Contents

---

*PDF viewers: These page numbers refer to the printed version of this document. Use the PDF reader bookmarks tab for links to specific sections.*

<b>1. Introduction .....</b>	<b>1</b>
<b>2. Cautionary Statements.....</b>	<b>1</b>
<b>3. Initial Inspection .....</b>	<b>1</b>
<b>4. Quickstart .....</b>	<b>2</b>
<b>5. Overview.....</b>	<b>5</b>
<b>6. Specifications .....</b>	<b>6</b>
<b>7. Installation.....</b>	<b>8</b>
7.1 Installation Considerations.....	8
7.1.1 Transducer Position .....	8
7.1.2 Vent Tube .....	8
7.1.3 Appropriate Water Depth.....	9
7.1.4 Dislodging Bubbles.....	9
7.2 Installation Procedure .....	9
7.2.1 Lower to depth.....	9
7.2.2 Secure the Transducer.....	9
7.2.2.1 Tie Wrap/Tape.....	9
7.2.2.2 Split Mesh Cable Grip.....	10
7.2.3 Measure the Initial Elevation .....	10
7.2.4 Offset Calculation.....	10
7.3 Wiring .....	11
7.3.1 SDI-12 Datalogger Connections .....	11
7.3.2 RS-232 Connections .....	11
7.3.3 A150/CWS900.....	12
7.4 Programming.....	12
7.4.1 CRBasic Programming .....	12
7.4.2 Edlog Programming .....	13
<b>8. Operation.....</b>	<b>13</b>
8.1 Configuration .....	13
8.1.1 PC Connection Using the A200.....	14
8.1.1.1 Driver Installation .....	14
8.1.1.2 A200 Wiring.....	14
8.1.1.3 Powering the Sensor.....	15
8.1.1.4 Determining which COM Port the A200 has been Assigned .....	15
8.1.2 Device Configuration Utility (version 2.03 or higher).....	15
8.2 SDI-12 Commands.....	16
8.3 Measuring Multiple SDI-12 Sensors.....	17

<b>9. Maintenance .....</b>	<b>17</b>
9.1 Every Visit .....	18
9.2 Every Two to Three Years or on a Rotating Schedule .....	18

<b>10. Troubleshooting.....</b>	<b>18</b>
---------------------------------	-----------

## Appendices

<b>A. Importing <i>Short Cut</i> Code .....</b>	<b>A-1</b>
---	------------

A.1 Importing <i>Short Cut</i> Code into a Program Editor.....	A-1
A.1.1 CRBasic Datalogger.....	A-1
A.1.2 Edlog .....	A-2

<b>B. Example Programs.....</b>	<b>B-1</b>
---------------------------------	------------

B.1 CRBasic Programs .....	B-1
B.1.1 Example Program for CR200(X)-Series Datalogger.....	B-1
B.1.2 Example Program for CR1000 Datalogger .....	B-2
B.2 Example Program for CR10(X) Dataloggers .....	B-3

<b>C. Calibration Certificate.....</b>	<b>C-1</b>
--	------------

<b>D. SDI-12 Sensor Support.....</b>	<b>D-1</b>
--------------------------------------	------------

D.1 SDI-12 Command Basics .....	D-1
D.1.1 Address Query Command (!) .....	D-1
D.1.2 Change Address Command (aAb!) .....	D-1
D.1.3 Send Identification Command (aI!).....	D-2
D.1.4 Start Measurement Commands (aM!) .....	D-2
D.1.5 Aborting a Measurement Command .....	D-2
D.1.6 Send Data Command (aDv!).....	D-2
D.2 SDI-12 Transparent Mode.....	D-3
D.2.1 CR200(X) Series Datalogger Example .....	D-3
D.2.2 CR1000 Datalogger Example.....	D-4
D.3 Advanced SDI-12 Commands.....	D-5

<b>E. RS-232 Connection Via PC Terminal Software.....</b>	<b>E-1</b>
---	------------

## Figures

5-1. CS451 nose cone options .....	6
7-1. Transducer suspended with split mesh cable grip .....	10
7-2. A150 wired for CS451 pressure sensor and CWS900 connector .....	12
8-1. A200 Sensor-to-PC Interface .....	14
8-2. Connect screen .....	16
D-1. CR200(X) example of using the SDI-12 transparent mode to change the SDI-12 address from 0 to 1.....	D-4
D-2. CR1000 example of using the SDI-12 transparent mode to change the SDI-12 address from 3 to 1. Sensor is connected to control port 1.....	D-5
E-1. Terminal Emulator .....	E-2



## Tables

7-1.	SDI-12 Wiring .....	11
7-2.	RS-232 Wiring .....	11
8-1.	Factory Settings .....	13
8-2.	A200 Wiring .....	14
8-3.	SDI-12 Commands.....	17
D-1.	SDI-12 Command and Response Set .....	D-1
D-2.	SDI-12 Commands.....	D-3
E-1.	RS-232 Settings .....	E-1
E-2.	RS-232 Terminal Commands.....	E-2



# CS451/CS456 Submersible Pressure Transducer

---

## 1. Introduction

The CS451/CS456 Submersible Pressure Transducer provides pressure and temperature measurements. It uses the SDI-12 or RS-232 communications protocols to communicate with an SDI-12 or RS-232 recorder simplifying installation and programming. The CS450/CS455 can be used with an A150 desiccated case allowing the transducer to be connected to a CWS900 wireless sensor or prewired enclosure.

## 2. Cautionary Statements

- READ AND UNDERSTAND the *Precautions* section at the front of this manual.
- Sensor will be damaged if it is encased in frozen liquid.
- Although the CS451/CS456 is rugged, it is also a highly precise scientific instrument and should be handled as such. There are no user-serviceable parts and any attempt to disassemble the device will void the warranty.
- Dropping the instrument or allowing it to “free fall” down a well may damage the transducer.
- Never suspend the CS451/CS456 from the connections at the top end of the cable. Sharp bends or excessive pinching of the cable can cause damage and may pinch off the vent tube causing measurement errors.
- Confirm the compatibility of the sensor and cable to non-water environments before installation.
- The CS456 instead of the CS451 should be used in harsh water applications, including salt water.

## 3. Initial Inspection

- Upon receipt of the CS451/CS456, inspect the packaging for any signs of shipping damage and, if found, report the damage to the carrier in accordance with policy. The contents of the package should also be inspected and a claim filed if any shipping related damage is discovered.
- The model number and pressure range is etched on the housing and the cable length is printed on the label near the connection end of the cable. Check this information against the shipping documentation to ensure that the expected product was received.
- Ensure that the desiccant tube is attached to the vent tube on the cable. The desiccant should be blue; replace if it is another color.

## 4. Quickstart

*Short Cut* is an easy way to program your datalogger to measure the sensor and assign datalogger wiring terminals. The following procedure shows using *Short Cut* to program the CS451/CS456.


1. Install *Short Cut* by clicking on the install file icon. Get the install file from either [www.campbellsci.com](http://www.campbellsci.com), the ResourceDVD, or find it in installations of *LoggerNet*, *PC200W*, *PC400*, or *RTDAQ* software.




2. The *Short Cut* installation should place a *Short Cut* icon on the desktop of your computer. To open *Short Cut*, click on this icon.




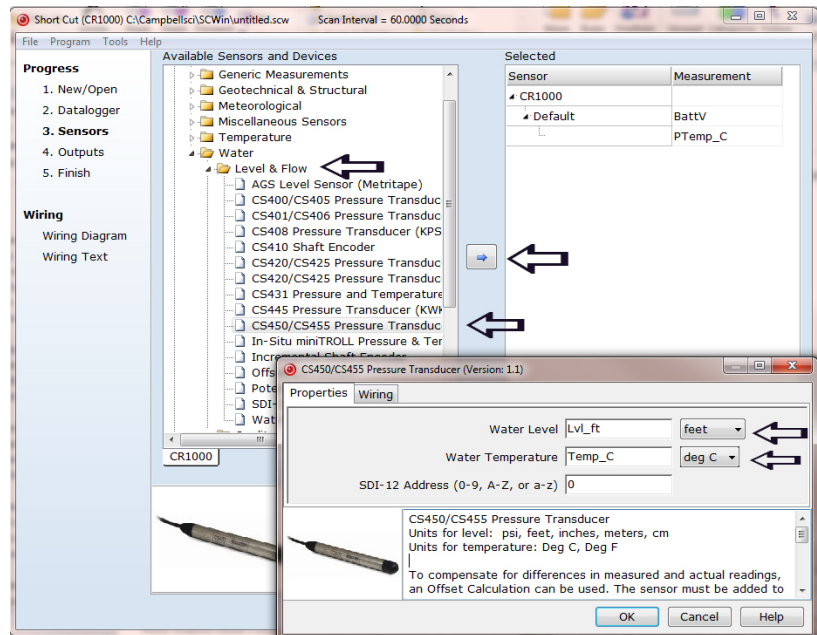
3. When *Short Cut* opens, select **New Program**.

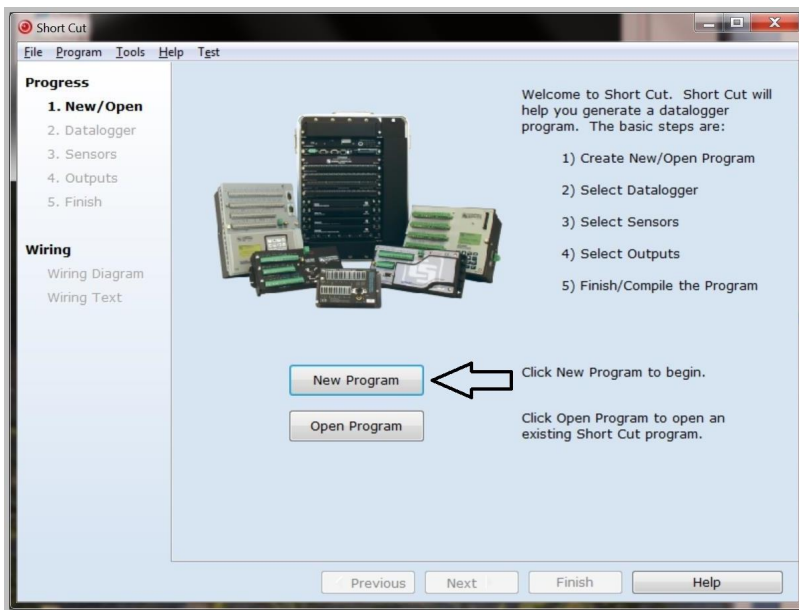


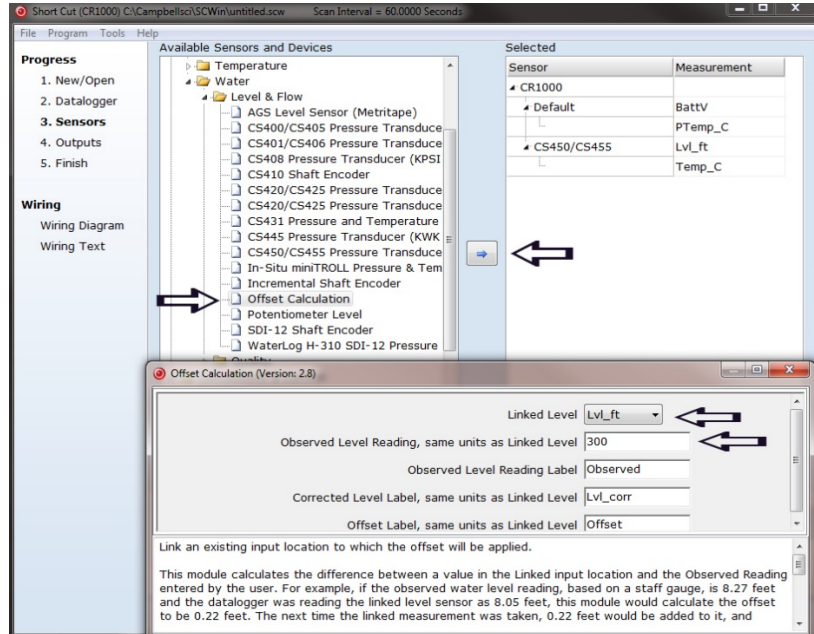
4. Select **Datalogger Model** and **Scan Interval** (60 second or higher scan interval is recommended). Click **Next**.

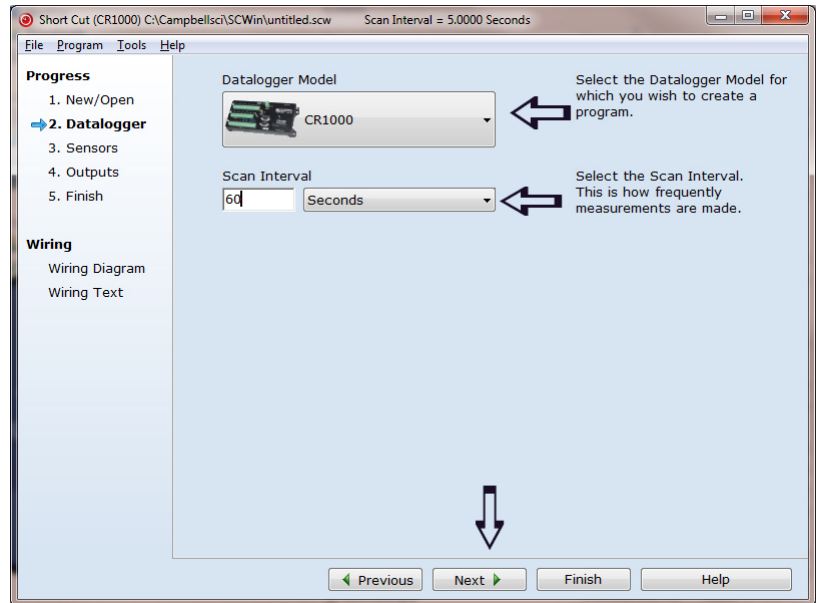


5. Under the **Available Sensors and Devices** list, select the **Sensors | Water | Level & Flow** folder. Select **CS450/CS455 Pressure Transducer**, click  to move the selection to the **Selected** device window. Water level defaults to feet and temperature defaults to degrees Celsius. These can be changed by clicking the **Water Level** or **Temperature** box and selecting a different option. Typically, the default SDI-12 address of 0 is used.



6. Under the **Available Sensors and Devices** list, select the **Sensors | Water | Level & Flow** folder. Select **Offset Calculation**, click  to move the selection to the **Selected** device window, then select **Lvl\_ft** for the **Linked Level** and enter the initial water level in the **Observed Level Reading** box.



7. After selecting the sensor and offset calculation, click at the left of the screen on **Wiring Diagram** to see how the sensor is to be wired to the datalogger. The wiring diagram can be printed out now or after more sensors are added.

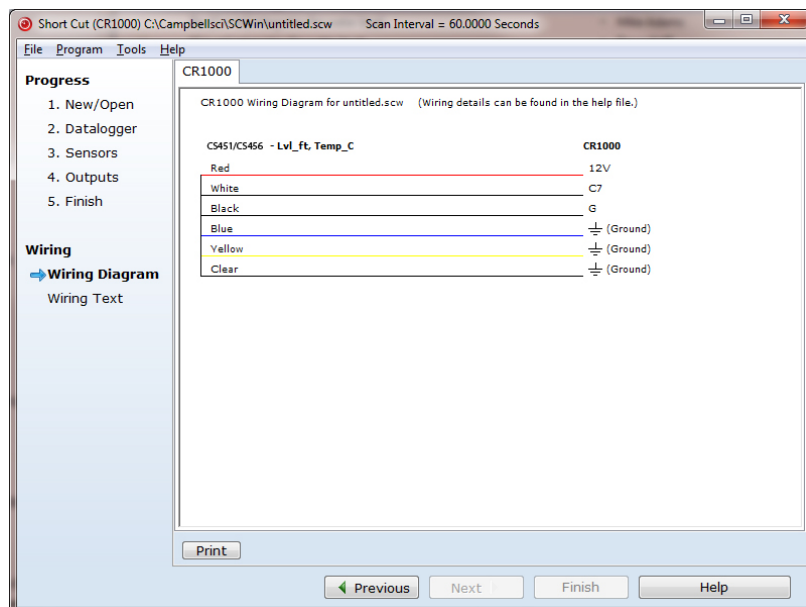

8. Select any other sensors you have, then finish the remaining *Short Cut* steps to complete the program. The remaining steps are outlined in *Short Cut Help*, which is accessed by clicking on **Help | Contents | Programming Steps**.
9. If *LoggerNet*, *PC400*, or *PC200W* is running on your PC, and the PC to datalogger connection is active, you can click **Finish** in *Short Cut* and you will be prompted to send the program just created to the datalogger.
10. If the sensor is connected to the datalogger, as shown in the wiring diagram in step 6, check the output of the sensor in the datalogger support software data display to make sure it is making reasonable measurements.

## 5. Overview

The CS451/CS456 pressure transducer provides a reliable, accurate pressure/level measurement that is fully temperature compensated. Its 24 bit A/D has simultaneous 50/60 Hz rejection and automatic calibration for each measurement.

A number of additional advanced measurement techniques are employed to harness the best possible performance available from today's state-of-the-art pressure transducer technology. The transducer reverts to a low power sleep state between measurements. A series of measurements are performed yielding a temperature and pressure value. This measurement cycle takes less than 1.5 second. The transducer can also be configured to output pressure only in less than 1 second. The measurement cycle is activated using SDI-12 or RS-232 commands.

The transducer consists of a piezoresistive sensor housed in a 316L stainless-steel (CS451) or titanium (CS456) package to enhance reliability. The rugged construction makes the CS451/CS456 suitable for water level measurement in irrigation applications, water wells, lakes, streams, and tanks. The titanium package of the CS456 makes it ideal for salt water or other harsh environments. The cable incorporates a vent tube to compensate for atmospheric pressure fluctuations and the jacket is made of rugged Hytrel®, designed to remain flexible and tough, even under harsh environmental conditions.

The CS451/CS456 has two communication options: SDI-12 or RS-232. The CS451/CS456 is shipped from the factory with both communications options enabled; there is no configuration required. As an SDI-12 sensor, the CS451/CS456 is shipped with an address of 0.

Two values are output by the CS451/CS456 — pressure/level and temperature. The CS451/CS456 is shipped from the factory to output pressure in psig and temperature in degrees Celsius.

The CS451/CS456 has three nose cone options. FIGURE 5-1 shows the nose cone options. The weighted nose cone makes the transducer easier to submerge to depth. The 1/4 inch NPT nose cone allows the transducer to be used in closed-pipe applications. Nose cones can be switched out later.

The -L in the transducer's model name indicates user-specified cable length.



FIGURE 5-1. CS451 nose cone options

## 6. Specifications

### Features:

- Output acceptable for recording devices with SDI-12 or RS-232 capability including Campbell Scientific dataloggers
- Quality construction that ensures product reliability
- Rugged stainless steel or titanium case that protects piezoresistive sensor
- Fully temperature compensated
- Low power sleep state between measurements that reduces power consumption
- Weighted nose cone offered that adds 0.2 kg (7.4 oz) to the transducer's weight. Additional weight makes submersion of the transducer easier
- Compatible with Campbell Scientific CRBasic dataloggers: CR200(X) series, CR800 series, CR1000, CR3000, and CR5000. Also compatible with Edlog dataloggers: CR500, CR510, CR10(X), and CR23X

**Power Requirements:** 5 to 18 Vdc

**Power Consumption:** Quiescent current < 50  $\mu$ A  
Measurement/Communication Current: 8 mA for 1-s measurement  
Maximum Peak Current: 40 mA

**Measurement Time:** Less than 1.5 s

**Outputs:** SDI-12 (version 1.3) 1200 bps  
RS-232 9600 bps



**Measurement Ranges:**

Pressure (psig)	Pressure (kPa)	Depth of fresh water
0 to 2.9	0 to 20	0 to 2 m (6.7 ft)
0 to 7.25	0 to 50	0 to 5.1 m (16.7 ft)
0 to 14.5	0 to 100	0 to 10.2 m (33.4 ft)
0 to 29	0 to 200	0 to 20.4 m (67 ft)
0 to 72.5	0 to 500	0 to 50.9 m (167 ft)
0 to 145	0 to 1000	0 to 102 m (334.5 ft)

**Accuracy:**  $\pm 0.1\%$  full scale range TEB\* or  
 $\pm 0.05\%$  full scale range TEB\*\*

**Resolution:** 0.0035% full scale range

**Overpressure:** 2x pressure range

**Dry Storage Temperature:**  $-10$  to  $80$  °C

**CAUTION**

Sensor will be damaged if it is encased in frozen liquid.

**Operating Temperature:**  $0$  to  $60$  °C

**Temperature Accuracy:**  $\pm 0.2$  °C

**Maximum Cable Length:**

**SDI-12 (one transducer  
connected to a single port):** ~475 m (1500 ft)

**SDI-12 (10 transducers  
connected to a single port):** 60 m (200 ft)

**RS-232:** 60 m (200 ft)

**Cable Type:** 5 Conductor, 26 AWG  
Hytrek Jacket

**Body Material:** CS451 – 316L Stainless Steel  
CS456 – Titanium

**Element Material:** CS451 – 316L Stainless Steel  
CS456 – Hastelloy

**Top Cone Material:** Delrin

**Length:** 213.36 mm (6.875 in)

**Diameter:** 21.34 mm (0.84 in)

**Distance from pressure sensor interface  
(black line etched on housing) to:**

**End of NPT fitting:** 2.54 cm (1 in)

**End of standard nose cone:** 2.3 cm (0.9 in)

**End of weighted nose cone:** 9.9 cm (3.9 in)

#### Air Gap

##### Standard and weighted

nose cone: 0.653 cm (0.257 in)

NPT fitting: 2.72 cm (1.07 in)

#### Weight:

CS451: 0.17 kg (0.37 lb)

CS456: 0.10 kg (0.23 lb)

Cable: 0.421 kg/m (0.283 lb/ft)

#### 25431 Split Mesh Grip

Accepts cable diameter: 4.57 to 6.35 mm (0.18 to 0.25 in)

Breaking Strength: (~300 lb)

\* Total Error Band (TEB) includes the combined errors due to nonlinearity, hysteresis, nonrepeatability, and thermal effects over the compensated temperature range, per ISA S51.1.

\*\* 0.05% full scale range accuracy not available in the 0 to 2.9 psig range.

## 7. Installation

If you are programming your datalogger with *Short Cut*, skip Section 7.3, *Wiring*, and Section 7.4, *Programming*. *Short Cut* does this work for you. See Section 4, *Quickstart*, for a *Short Cut* tutorial.

### 7.1 Installation Considerations

The CS451/CS456 is designed for water level measurements. Typical applications include agricultural water level/flow, water wells, lakes, streams, and tanks. If the device is to be installed in a liquid other than water or in contaminated water, check the compatibility of the wetted material. The CS456 should be used in harsh water applications, including salt water.

#### 7.1.1 Transducer Position

The CS451/CS456 can be installed in any position; however, when it leaves the factory it is tested in the vertical position. There will be an offset error if not installed vertically; contact Campbell Scientific for more information.

#### 7.1.2 Vent Tube

A vent tube incorporated in the cable vents the sensor diaphragm to the atmosphere. This eliminates the need to compensate for changes in barometric pressure. To prevent water vapor from entering the inner cavity of the sensor, the vent tube opening terminates inside a desiccant tube.

#### CAUTION

The desiccant tube is shipped with a black cap to cover the vent hole. This cap **MUST** be removed prior to installation.

Before installing the sensor, ensure the desiccant is blue; replace if not.

The desiccant tube must always be attached to the CS451/CS456.

### 7.1.3 Appropriate Water Depth

The CS451/CS456 must be installed below the water at a fixed depth. This depth should be chosen so the water pressure will never exceed the transducer's pressure range (twice its pressure range).

#### CAUTION

The output reading will not be correct, and the transducer can be damaged if pressure is excessive (2 x full scale).

Pressure can be converted to feet of fresh water using the following simple equation:

$$1 \text{ psi} = 2.31 \text{ feet of water}$$

For example, the maximum depth with a pressure range of 0 to 7.25 psig is 16.748 feet of water.

### 7.1.4 Dislodging Bubbles

While submersing the transducer, air bubbles may become trapped between the pressure plate and the water surface, causing small offset errors until the bubbles dissolve. Dislodge these bubbles by gently shaking the CS451/CS456 while under water.

#### CAUTION

If bubbles are not removed by rotation and shaking underwater (or bleeding out the air in a closed system), the CS451/CS456 reading will drift lower by the distance of the gap as the bubbles are slowly dissolved into the water over time.

#### CAUTION

Hitting against the well casing or other solid surface could damage the transducer.

## 7.2 Installation Procedure

### 7.2.1 Lower to depth

Lower the transducer to an appropriate depth.

#### CAUTION

Do not drop the instrument or allow it to "free fall" down a well as this may damage the sensor.

With long drops, it may be necessary to use the weighted nose cone (option -WN).

### 7.2.2 Secure the Transducer

#### 7.2.2.1 Tie Wrap/Tape

The transducer body can be strapped with tie wraps or tape. Campbell Scientific offers cable ties (pn 7421) that can be used to secure and strain relief

the cable. If installing in a well, fasten the cable to the well head. Wrap the cable ties around the cable jacket.

---

**CAUTION**

Never suspend the CS451/CS456 from the connections at the top of the cable. Sharp bends or excessive pinching of the cable can cause damage and may pinch off the vent tube causing measurement errors.

---

#### **7.2.2.2 Split Mesh Cable Grip**

The 25431 Split Mesh Cable Grip can be used to center the cable and to provide a method of suspending the cable-reducing cable stretch. It is often recommended for use in wells. FIGURE 7-1 shows a transducer's cable suspended using the split mesh cable grip.



*FIGURE 7-1. Transducer suspended with split mesh cable grip*

#### **7.2.3 Measure the Initial Elevation**

Use a staff gauge (or other device) to measure the initial elevation of water. This value is used to calculate an offset that corrects the final measurement for errors due to zero offset or installation. SCWin will make the offset calculation. Refer to Section 7.2.4, *Offset Calculation*, if not using SCWin to calculate the offset.

After installation, several readings should be taken to ensure proper operations after installation.

#### **7.2.4 Offset Calculation**

The pressure created is directly proportional to the water column above the sensor. An offset is used to correct the final measurement to any error due to sensor zero offset or installation.

For example, if the correct elevation of the water, as measured by a staff gauge or other measurement device, is 2015.50 feet, and the CS451 provides a reading of 5.76 psig, then:

$$5.76 \text{ psig} \cdot 2.31 \text{ ft/psig} = 13.3056 \text{ ft.}$$

So, the offset is calculated:

$$2015.50 \text{ ft} - 13.3056 \text{ ft} = 2002.1944 \text{ ft}$$

This offset can be accounted for in the program instruction of the SDI-12 recorder.

## 7.3 Wiring

### NOTE

Power down your system before wiring the CS451/CS456. The shield wire plays an important role in noise emissions and susceptibility as well as transient protection.

### 7.3.1 SDI-12 Datalogger Connections

TABLE 7-1. SDI-12 Wiring				
Color	CS451/CS456 Function	CR800 CR5000 CR3000 CR1000	CR200(X) Series	CR510 CR23X CR10X
Red	+12 Vdc	12 V	Battery+	12 V
Black	Power Ground	G	G	G
White	SDI-12 Signal	*Control Port	C1/SDI-12	Control Port
Blue	GND	GND	G	G
Yellow	GND	GND	G	G
Clear	Shield	GND	G	G

\*dedicated SDI-12 port on CR5000

### 7.3.2 RS-232 Connections

TABLE 7-2. RS-232 Wiring			
Color	CS451/CS456 Function	Connection	RS-232 9-pin
Red	+12vdc	Power Source	
Black	Power Ground	Power Ground	
White	RS-232 Tx (Output)	Transmit	Pin 2 Rx (Input)
Blue	RS-232 Rx (Input)	Receive	Pin 3 Tx (Output)
Yellow	Digital Ground	Ground	Pin 5 GND
Clear	Shield GND	Ground	

### 7.3.3 A150/CWS900

The A150 desiccated case allows the CS451/CS456 to be connected to the CWS900 wireless sensor and then used in a wireless network. FIGURE 7-2 shows the CS451 wired to the A150's terminal block. The 26972 cable is included with the A150.

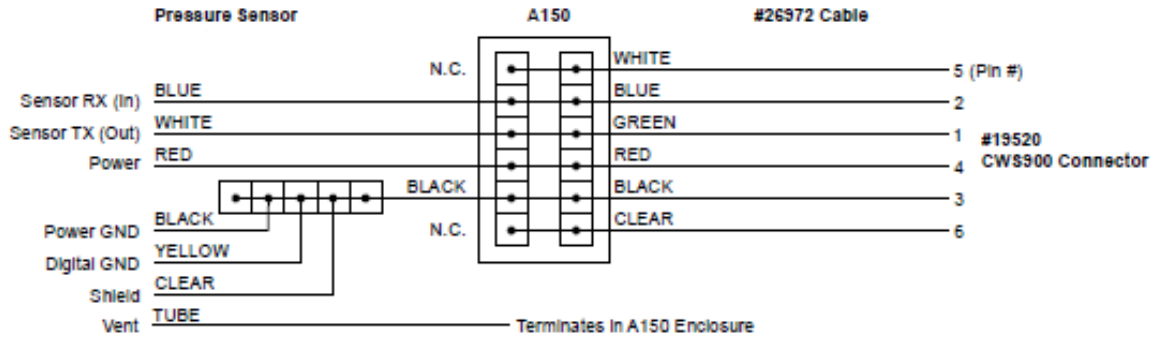


FIGURE 7-2. A150 wired for CS451 pressure sensor and CWS900 connector

## 7.4 Programming

*Short Cut* is the best source for up-to-date datalogger programming code. Programming code is needed,

- when creating a program for a new datalogger installation
- when adding sensors to an existing datalogger program

If your data acquisition requirements are simple, you can probably create and maintain a datalogger program exclusively with *Short Cut*. If your data acquisition needs are more complex, the files that *Short Cut* creates are a great source for programming code to start a new program or add to an existing custom program.

### NOTE

*Short Cut* cannot edit programs after they are imported and edited in *CRBasic Editor*.

A *Short Cut* tutorial is available in Section 4, *Quickstart*. If you wish to import *Short Cut* code into either *Edlog* or *CRBasic Editor* to create or add to a customized program, follow the procedure in Appendix A.1, *Importing Short Cut Code into a Program Editor*. Programming basics for *CRBasic* and *Edlog* dataloggers are provided in the following sections. Complete program examples for select dataloggers can be found in Appendix B, *Example Programs*.

### 7.4.1 CRBasic Programming

The **SDI12Recorder()** measurement instruction programs *CRBasic* dataloggers (CR200(X)-series, CR800-series, CR1000, CR3000, and CR5000) to measure the CS451/CS456 sensor. This instruction sends a request to the sensor to make a measurement and then retrieves the measurement from the sensor. See Section 8.2, *SDI-12 Commands*, for more information.

When using a CR200(X), the **SDI12Recorder()** instruction has the following syntax:

**SDI12Recorder**(*Destination, OutString, Multiplier, Offset*)

For the other CRBasic dataloggers, the **SDI12Recorder()** instruction has the following syntax:

**SDI12Recorder**(*Destination, SDIPort, SDIAddress, "SDICommand", Multiplier, Offset*)

## 7.4.2 Edlog Programming

Edlog dataloggers read the CS451/CS456 using the **SDI-12 Recorder (P105)** instruction.

Please note that Edlog only allocates one input location for the **SDI-12 Recorder (P105)** instruction. Two input locations are required for the SDI-12 **M!** command. The additional input locations need to be inserted manually using the Input Location Editor. To get into the **Input Location Editor**, select **Edit/Input Labels** or press the **F5** key. Once in the **Input Location Editor**, do the following:

1. Choose **Edit/Insert Block**.
2. After the **Insert Block** dialog box appears, type in a base name for the input locations. Each input location will have the base name with an underscore and a consecutive number.
3. In the **Start Address** field, type in the number of the first input location.
4. In the **Number of InLocs** field, type in 2 and select **OK**.

# 8. Operation

## 8.1 Configuration

TABLE 8-1 shows default settings of the CS451/CS456.

TABLE 8-1. Factory Settings	
SDI-12 Address	0
RS-232 Baud Rate	9600
Pressure/Level Units	psig
Temperature Units	Celsius

Communicating with the CS451/CS456 requires the sensor to be either connected to a PC or to an SDI-12 recorder. The sensor typically connects to a PC via the A200 sensor to PC interface. Many SDI-12 recorders allow communication to the sensor via a terminal screen. Configurable settings can be changed via SDI-12 commands or by using Campbell Scientific's software *Device Configuration Utility*.

### 8.1.1 PC Connection Using the A200

The A200 or another device is required to connect the CS451/CS456 to a PC. This allows sensor settings to be changed via our *Device Configuration Utility*.

#### 8.1.1.1 Driver Installation

If the A200 has not been previously plugged into your PC and your PC operating system is not Windows 7, the A200 driver needs to be loaded onto your PC.

#### NOTE

Drivers should be loaded before plugging the A200 into the PC.

The A200 drivers can be downloaded, at no charge, from:  
[www.campbellsci.com/downloads](http://www.campbellsci.com/downloads).

#### 8.1.1.2 A200 Wiring

One end of the A200 has a terminal block while the other end has a type B female USB port. The terminal block provides 12V, G, TX, and RX terminals for connecting the sensor (see FIGURE 8-1 and TABLE 8-2). A data cable (pn 17648) ships with the A200. This cable has a USB type-A male connector that attaches to a PC's USB port, and a type B male connector that attaches to the A200's USB port.



FIGURE 8-1. A200 Sensor-to-PC Interface

TABLE 8-2. A200 Wiring		
Color	Sensor Cable Label	A200 Terminal
Red	12V	+12Vdc
Black	G	G
White	C	Tx
Blue	G	Rx
Yellow	G	G
Clear	Signal Ground	G



#### 8.1.1.3 Powering the Sensor

The A200 provides power to the sensor when it is connected to a PC's USB port. An internal DC/DC converter boosts the 5 Vdc supply from the USB connection to a 12 Vdc output is required to power the sensor.

#### 8.1.1.4 Determining which COM Port the A200 has been Assigned

When the A200 driver is loaded, the A200 is assigned a COM port number. This COM port number is needed when using the *Device Configuration Utility* or a PC terminal software such as *HyperTerminal*.

Often, the assigned COM port will be the next port number that is free. However, if other devices have been installed in the past (some of which may no longer be plugged in), the A200 may be assigned a higher COM port number.

To check which COM port has been assigned to the A200, watch for the appearance of a new COM port in the list of COM ports offered in the software package (e.g., *LoggerNet*) before and after the installation, or look in the Windows Device Manager list under the ports section (access via the control panel).

### 8.1.2 Device Configuration Utility (version 2.03 or higher)

The *Device Configuration Utility* allows you to change the settings of the CS451/CS456. *Device Configuration Utility* is shipped on the Campbell Scientific ResourceDVD included with the CS451/CS456.

To use *Device Configuration Utility*, the transducer needs to be connected to the PC via the A200 (see Section 8.1.1, *PC Connection Using the A200*). After installing *Device Configuration Utility* and connecting the transducer to the PC, select CS451 from the Device Type list on the left column of the screen.

In the PC Serial Port box, select the COM port that was assigned to the A200 (see Section 8.1.1.4, *Determining which COM Port the A200 has been Assigned*). Click on the **Connect** button to enable communication with the sensor. Once successfully connected, the screen should look like FIGURE 8-2.

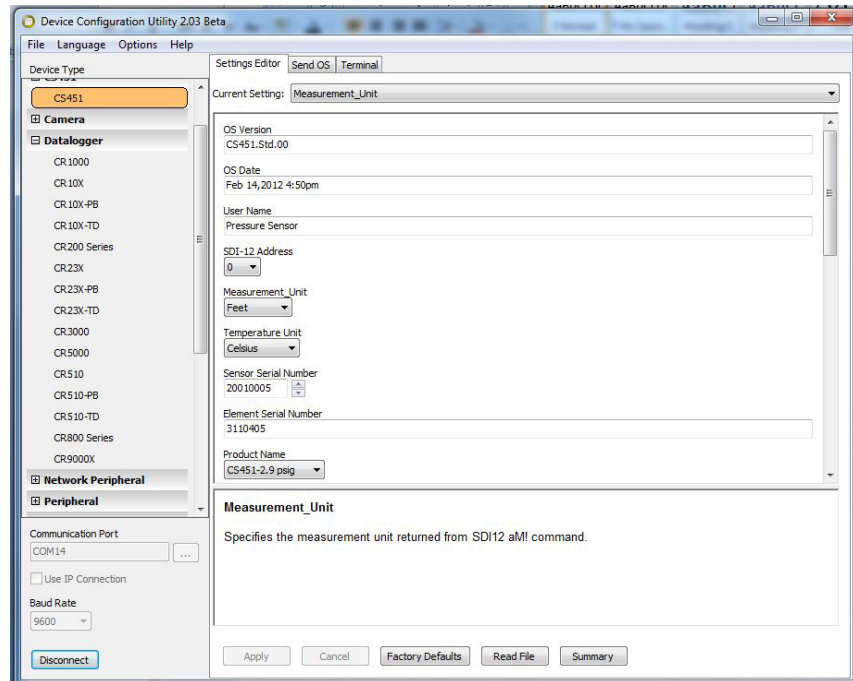


FIGURE 8-2. Connect screen

There are three settings that can be changed: SDI-12 address, Pressure/Level Units, and Temperature Units. Double-click on the window of the units to be changed. This will open a pick menu box. Select the desired units and **Apply** the changes.

## 8.2 SDI-12 Commands

### NOTE

This section briefly describes using the SDI-12 commands. Additional SDI-12 information is available at Appendix D, *SDI-12 Sensor Support*, [www.sdi-12.org](http://www.sdi-12.org), or [www.youtube.com/user/CampbellScientific](http://www.youtube.com/user/CampbellScientific).

The CS451/CS456 uses an SDI-12 compatible hardware interface and supports a subset of the SDI-12 commands. The most commonly used command is the **aM!** command, issued by the datalogger, where *a* represents the sensor address. The communication sequence begins with the datalogger waking the sensor and issuing the **aM!** command. The transducer responds to the datalogger indicating that two measurements will be ready within two seconds. Subsequent communications handle data reporting from the sensor to the datalogger.

The SDI-12 protocol has the ability to support various measurement commands. The CS451/CS456 supports the commands that are listed in TABLE 8-3.

**TABLE 8-3. SDI-12 Commands**

<b>SDI-12 Command</b>	<b>Command Function</b>	<b>Values Returned</b>
aM!	Configured settings	Pressure/Level, Temperature
aM1!	PSIG, °C	Pressure, Temperature
aM2!	PSIG, °F	Pressure, Temperature
aM3!	kPa, °C	Pressure, Temperature
aM4!	kPa, °F	Pressure, Temperature
aM5!	Sensor's Serial Number	Serial Number
aM6!	Ohms, ohms, °C	$\Delta R$ , Rb, Temperature
aM7!	Configured settings (provides data in less than 0.8 seconds)	Pressure/Level
aM8!	Configured settings (provides average of data based on user selected samples)	Pressure/Level, Temperature

As measurement data is transferred between the probe and datalogger digitally, there are no offset errors incurred with increasing cable length as seen with analog sensors. However, with increasing cable length, there is still a point when digital communications break down, resulting in either no response or excessive SDI-12 retries and incorrect data due to noise problems. (Using SDI-12 commands like **aMC!**, which adds a CRC check, can significantly improve incorrect data issues.)

### 8.3 Measuring Multiple SDI-12 Sensors

Up to ten CS451/CS456 sensors or other SDI-12 sensors can be connected to a single datalogger control port. Each SDI-12 device must have a unique SDI-12 address of 0 and 9, A to Z, or a to z. See Appendix D, *SDI-12 Sensor Support*, for more information.

## 9. Maintenance

Campbell Scientific recommends that the CS451/CS456 be factory recalibrated and checked every 24 months. Before a CS451/CS456 sensor is sent to Campbell Scientific, the customer must get an RMA (returned material authorization) number, and fill out the Declaration of Hazardous Material and Decontamination form.

The CS451/CS456 has no user-serviceable parts. Cable can be damaged by abrasion, rodents, sharp objects, twisting, crimping or crushing, and pulling. Take care during installation and use to avoid cable damage. If a section of cable is damaged, it is recommended that you send your sensor back to replace the bale harness assembly.

Periodic evaluation of the desiccant is vital for keeping the vent tube dry. The CS451/CS456 ships with the desiccant tube attached. To assess the effectiveness of the desiccant, use one of the following:

- The desiccant in the tube changes color from blue to pink when the drying power is lost.
- The Enclosure Accessory Humidity Indicator Card (pn 28878).

## 9.1 Every Visit

- Collect data.
- Visually inspect wiring and physical conditions.
- Check indicating desiccant or enclosure humidity indicator; service if necessary.
- Check battery condition (inspect physical appearance and use a keyboard display, PDA, or laptop to view the battery voltage).
- Check all sensor readings; adjust transducer offsets if necessary.
- Check recent data.

## 9.2 Every Two to Three Years or on a Rotating Schedule

- Send the CS451/CS456 in for inspection.

# 10. Troubleshooting

The most common causes for erroneous pressure transducer data include:

- poor sensor connections to the datalogger
- damaged cables
- damaged transducers
- moisture in the vent tube

*Problem:*

Unit will not respond when attempting serial communications.

*Suggestion:*

Check the power (red is +V and black is ground) and signal (white is SDI-12 data) lines to ensure proper connection to the datalogger. Check the datalogger program to ensure that the same port the SDI-12 data line is connected to is specified in the measurement instruction.

*Problem:*

Transducer appears to be operating properly but data shows a periodic or cyclic fluctuation not attributable to water level changes.

*Suggestion:*

A kinked or plugged vent tube will not effectively vent a gauge pressure (Vented) type of device. Normal changes in barometric pressure will appear as water level fluctuations and these types of errors are typically on the order of 1 foot of water level. If the desiccant chamber has not been properly maintained, water may have condensed in the vent tube and the device should be returned to the factory for service.



# ***Appendix A. Importing Short Cut Code***

---

This tutorial shows:

- How to import a *Short Cut* program into a program editor for additional refinement
- How to import a wiring diagram from *Short Cut* into the comments of a custom program

## **A.1 Importing *Short Cut* Code into a Program Editor**

*Short Cut* creates files that can be imported into either *CRBasic Editor* or *Edlog* program editor. These files normally reside in the C:\campbellsci\SCWin folder and have the following extensions:

- .DEF (wiring and memory usage information)
- .CR2 (CR200(X) datalogger code)
- .CR1 (CR1000 datalogger code)
- .CR8 (CR800 datalogger code)
- .CR3 (CR3000 datalogger code)
- .CR5 (CR5000 datalogger code)
- .DLD (contain code for CR10(X), CR23X, CR500, or CR510 dataloggers)

The following procedures show how to import these files for editing.

### **A.1.1 CRBasic Datalogger**

Use the following procedure to import *Short Cut* code into *CRBasic Editor* (CR200(X), CR1000, CR800, CR3000, CR5000 dataloggers).

1. Create the *Short Cut* program following the procedure in Section 4, *Quickstart*. Finish the program and exit *Short Cut*. Make note of the file name used when saving the *Short Cut* program.
2. Open *CRBasic Editor*.
3. Click **File | Open**. Assuming the default paths were used when *Short Cut* was installed, navigate to C:\CampbellSci\SCWin folder. The file of interest has a “.CR2”, “.CR1”, “.CR8”, “.CR3”, or “.CR5” extension, for CR200(X), CR1000, CR800, CR3000, or CR5000 dataloggers, respectively. Select the file and click **Open**.
4. Immediately save the file in a folder different from \Campbellsci\SCWin, or save the file with a different file name.

---

#### **NOTE**

Once the file is edited with *CRBasic Editor*, *Short Cut* can no longer be used to edit the datalogger program. Change the name of the program file or move it, or *Short Cut* may overwrite it next time it is used.

---

5. The program can now be edited, saved, and sent to the datalogger.
6. Import wiring information to the program by opening the associated .DEF file. Copy and paste the section beginning with heading “-Wiring for CRXXX-” into the CRBasic program, usually at the head of the file. After pasting, edit the information such that a ' character (single quotation mark) begins each line. This character instructs the datalogger compiler to ignore the line when compiling the datalogger code.

## A.1.2 Edlog

Use the following procedure to import *Short Cut* code into the *Edlog* program editor (CR10(X), CR500, CR510, and CR23X dataloggers).

1. Create the *Short Cut* program following the procedure in Section 4, *Quickstart*. Finish the program and exit *Short Cut*. Make note of the file name used when saving the *Short Cut* program.
2. Open *Edlog*.
3. Click **File | Document DLD File**. Assuming the default paths were used when *Short Cut* was installed, navigate to C:\CampbellSci\SCWin folder. The file of interest has a “.DLD” extension. Select the file and click **Open**. The .dld file, which is a type of ASCII machine code, is imported, documented, and, when saved, given a “.CSI” extension.
4. Immediately save the file in a folder different from \Campbellsci\SCWin, or save the file with a different file name.

---

### NOTE

Once the file is edited with *Edlog*, *Short Cut* can no longer be used to edit the program. Change the name of the program file or move it, or *Short Cut* may overwrite it.

---

5. The program can now be edited, saved, and sent to the datalogger.
6. Import wiring information to the program by opening the associated .DEF file. Copy and paste the section beginning with heading “-Wiring for CRXXX-” into the Edlog program, usually at the head of the file. After pasting, edit the information such that a ; (semicolon) begins each line, which instructs the datalogger compiler to ignore the line when compiling the datalogger code.



# ***Appendix B. Example Programs***

---

## **B.1 CRBasic Programs**

### **B.1.1 Example Program for CR200(X)-Series Datalogger**

```
'CR200(X) Series

'Declare the variable for the water level measurement
Public CS451(2)

'Rename the variable names
Alias CS451(1)=Level
Alias CS451(2)=Temp_C

'Define a data table for 60 minute maximum and minimums
DataTable(Hourly,True,-1)
  DataInterval(0,60,Min)
  Maximum(1,Level,0,0)
  Minimum(1,Level,0,0)
  Maximum(1,Temp_C,0,0)
  Minimum(1,Temp_C,0,0)
EndTable

'Read sensor every 60 seconds
BeginProg
  Scan(60,sec)

  'Code for SDI-12 measurements:
  SDI12Recorder(CS451,OM!,1,0)

  'Call the data table:
  CallTable(Hourly)

  NextScan
EndProg
```

## B.1.2 Example Program for CR1000 Datalogger

```
'CR1000 Series Datalogger

'Declare the variable for the water level measurement
Public CS451(2)

'Rename the variable names
Alias CS451(1)=Level
Alias CS451(2)=Temp_C

'Define a data table for 60 minute maximum and minimums
DataTable(Hourly,True,-1)
  DataInterval(0,60,Min,10)
  Maximum(1,Level,FP2,0,0)
  Minimum(1,Level,FP2,0,0)
  Maximum(1,Temp_C,FP2,0,0)
  Minimum(1,Temp_C,FP2,0,0)
EndTable

'Read sensor every 60 seconds
BeginProg
  Scan(60,sec,1,0)

  'Code for SDI-12 measurements:
  SDI12Recorder(CS451,1,"0","M!",1,0)

  'Call the data table:
  CallTable(Hourly)

  NextScan
EndProg
```

## B.2 Example Program for CR10(X) Dataloggers

Below is a portion of a CR10X program that measures the CS451/CS456.

### NOTE

The instructions below do not store data in final storage. Instruction 92, Instruction 77, and processing instructions such as Instruction 70 are required to store the data permanently.

```
;{CR10X}
;
*Table 1 Program
01: 60      Execution Interval (seconds)

1: SDI-12 Recorder (P105)
  1: 0      SDI-12 Address
  2: 0      Start Measurement (aM0!)
  3: 1      Port ;this is where the white wire is connected
  4: 1      Loc[Data_1      ]
  5: 1.0    Mult
  6: 0.0    Offset

*Table 2 Program
02: 0.000   Execution Interval (seconds)

*Table 3 Subroutines

End Program
```

After Instruction 105 is executed, the input location called “Data\_1” will hold the measured pressure, reported in PSI, and the input location called Data\_2 will hold the measured temperature, in degrees Celsius. The results can be further processed by the datalogger. Note that Port 1 specifies that the SDI-12 data line is to be connected to the Port C1.



## ***Appendix C. Calibration Certificate***

---

Each CS451/CS456 has been calibrated to meet printed accuracy specification at multiple temperature and pressure ranges. If additional verification is required, a Calibration Certificate can be purchased for each CS451/CS456 Submersible Pressure Transducer.

The Instrument Data Report provides a list of the pressure and temperature at which the sensor was tested.

Pressure [kPa] is the pressure applied (listed in kilopascals) to the sensor. Temperature [°C] is the temperature inside the test chamber at the time of testing. Pressure After [kPa] represents the resulting measurement output by the CS451/CS456 at the give pressure and temperature. Finally, Deviation After [%F.S.], provides the difference between the actual pressure applied to the sensor and the pressure measurement output by the sensor. This value is listed as a percentage of the Full Scale range of the sensor.

When a CS451/CS456 is returned to Campbell Scientific for calibration, the sensor will be returned with an Instrument Data Report. This report will include values in the Pressure Before [kPa] column. These values represent the measured pressure the sensor returns at the specified pressure and temperature, BEFORE calibration.



# Appendix D. SDI-12 Sensor Support

## D.1 SDI-12 Command Basics

SDI-12 commands have three components:

*Sensor address (a)* – a single character, and is the first character of the command. The default address of zero (0) can be used unless multiple sensors are connected to the same port.

*Command body (e.g., M1)* – an upper case letter (the “command”) followed by alphanumeric qualifiers.

*Command termination (!)* – an exclamation mark.

An active sensor responds to each command. Responses have several standard forms and terminate with <CR><LF> (carriage return – line feed). Standard SDI-12 commands supported by the CS451/CS456 are listed in TABLE D-1. Appendix D.3 provides advanced commands.

TABLE D-1. SDI-12 Command and Response Set		
Name	Command	Response
Acknowledge Active	a!	a<CR><LF>
Send Identification	a!	allccccccmmmmmmvvvxxx...xx<CR><LF>
Change Address	aAb!	b<CR><LF>
Address Query	?!	a<CR><LF>
Start Measurement	aM!	atttn<CR><LF>
Send Data	aD0!	a<values><CR><LF>
Start Verification	aV!	atttn

### D.1.1 Address Query Command (?!)

Command ?! requests the address of the connected sensor. The sensor replies to the query with the address, *a*.

### D.1.2 Change Address Command (aAb!)

Sensor address is changed with command **aAb!**, where *a* is the current address and *b* is the new address. For example, to change an address from 0 to 2, the command is **0A2!**. The sensor responds with the new address *b*, which in this case is 2.

### D.1.3 Send Identification Command (**aI!**)

Sensor identifiers are requested by issuing command **aI!**. The reply is defined by the sensor manufacturer, but usually includes the sensor address, SDI-12 version, manufacturer's name, and sensor model information. Serial number or other sensor specific information may also be included.

An example of a response from the **aI!** command is:

*013CSI451.Std.01\_12345678*

Where:

SDI-12 version = 1.3

Manufacturer = CSI

Sensor model = 451

Operating System = .Std 01

Sensor serial number = 12345678

### D.1.4 Start Measurement Commands (**aM!**)

A measurement is initiated with **M!** commands. The response to each command has the form *attnn*, where

*a* = sensor address

*ttt* = time, in seconds, until measurement data are available

*nn* = the number of values to be returned when one or more subsequent **D!** commands are issued.

### D.1.5 Aborting a Measurement Command

A measurement command (**M!**) is aborted when any other valid command is sent to the sensor.

### D.1.6 Send Data Command (**aDv!**)

This command requests data from the sensor. It is normally issued automatically by the datalogger after measurement commands **aMv!**. In transparent mode, the user asserts this command to obtain data. If the expected number of data values are not returned in response to an **aD0!** command, the datalogger issues **aD1!**. TABLE D-2 shows the values returned when using the send data command.



TABLE D-2. SDI-12 Commands

SDI-12 Command	Command Function	Values Returned
aD!	Configured settings	Pressure/Level, Temperature
aD1!	psig, °C	Pressure, Temperature
aD2!	psig, °F	Pressure, Temperature
aD3!	kPa, °C	Pressure, Temperature
aD4!	kPa, °F	Pressure, Temperature
aD5!	Sensor's Serial Number	Serial Number
aD6!	Ohms, ohms, °C	$\Delta R$ , Rb, Temperature
aD7!	Configured settings (provides data in less than 0.8 seconds)	Pressure/Level
aD8!	Configured settings (provides average of data based on user selected samples)	Pressure/Level, Temperature

## D.2 SDI-12 Transparent Mode

System operators can manually interrogate and enter settings in probes using transparent mode. Transparent mode is useful in troubleshooting SDI-12 systems because it allows direct communication with probes. Datalogger security may need to be unlocked before transparent mode can be activated.

Transparent mode is entered while the PC is in telecommunications with the datalogger through a terminal emulator program. It is easily accessed through Campbell Scientific datalogger support software, but is also accessible with terminal emulator programs such as Windows HyperTerminal. Datalogger keyboards and displays cannot be used.

The terminal emulator is accessed by navigating to the Datalogger menu in *PC200W*, the Tools menu in *PC400*, or the Datalogger menu in the *Connect* screen of *LoggerNet*.

The following examples show how to use *LoggerNet* software to enter transparent mode and change the SDI-12 address of a CS451/CS456 sensor. The same steps are used to enter transparent mode with *PC200W* and *PC400* software after accessing the terminal emulator as previously described.

### D.2.1 CR200(X) Series Datalogger Example

1. Connect a single CS451/CS456 to the CR200(X) (see TABLE 7-1).
2. In the *LoggerNet Connect* screen navigate to the **Datalogger** menu and select **Terminal Emulator**. The terminal emulator window will open. In the **Select Device** menu, located in the lower left-hand side of the window, select the CR200Series station.

3. Click on the **Open Terminal** button.
4. Press the <enter> key until the datalogger responds with the *CR2XX>* prompt. At the *CR2XX>* prompt, make sure the **All Caps Mode** box is checked and enter the command **SDI12** <enter>. The response *SDI12>* indicates that the CS451/CS456 is ready to accept SDI-12 commands.
5. To query the CS451/CS456 for its current SDI-12 address, key in **?!<enter>** and the CS451/CS456 will respond with its SDI-12 address. If no characters are typed within 60 seconds, then the mode is exited. In that case, simply enter the command **SDI12** again and press <enter>.
6. To change the SDI-12 address, key in **aAb!<enter>**, where *a* is the current address from the above step and *b* is the new address (see FIGURE D-1). The CS451/CS456 will change its address and the datalogger will respond with the new address. To exit SDI-12 transparent mode select the **Close Terminal** button.

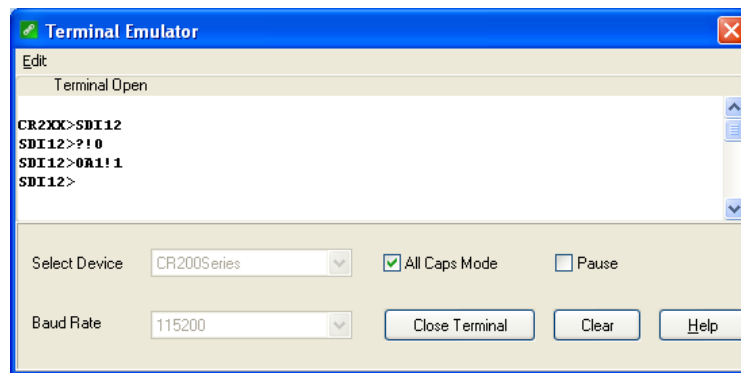


FIGURE D-1. CR200(X) example of using the SDI-12 transparent mode to change the SDI-12 address from 0 to 1.

## D.2.2 CR1000 Datalogger Example

1. Connect a CS451/CS456 to the CR1000 (see TABLE 7-1).
2. In the *LoggerNet Connect* screen, navigate to the **Datalogger** menu and select **Terminal Emulator**. The terminal emulator window will open. In the **Select Device** menu, located in the lower left-hand side of the window, select the CR1000 station.
3. Click on the **Open Terminal** button.
4. Press the <enter> key until the datalogger responds with the *CR1000>* prompt. At the *CR1000>* prompt, make sure the **All Caps Mode** box is checked and enter the command **SDI12** <enter>. At the *Enter Cx Port 1, 3, 5, or 7* prompt, key in the control port number where the CS451/CS456 is connected and press <enter>. The response *Entering SDI12 Terminal* indicates that the CS451/CS456 is ready to accept SDI-12 commands.
5. To query the CS451/CS456 for its current SDI-12 address, key in **?!<enter>** and the CS451/CS456 will respond with its SDI-12 address. If no

characters are typed within 60 seconds, then the mode is exited. In that case, simply enter the command SDI12 again, press <enter>, and key in the correct control port number when prompted.

6. To change the SDI-12 address, key in **aAb!** <enter>, where *a* is the current address from the above step and *b* is the new address (see FIGURE D-2). The CS451/CS456 will change its address and the datalogger will respond with the new address. To exit SDI-12 transparent mode, select the **Close Terminal** button.

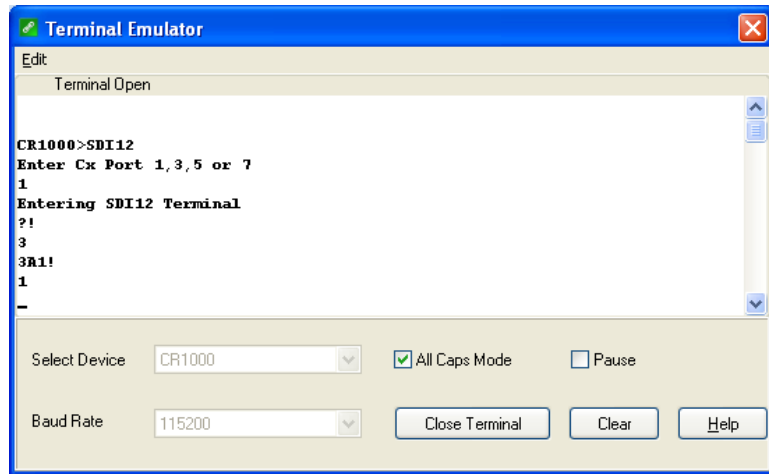


FIGURE D-2. CR1000 example of using the SDI-12 transparent mode to change the SDI-12 address from 3 to 1. Sensor is connected to control port 1.

## D.3 Advanced SDI-12 Commands

Extended SDI-12 commands can be used to configure the CS451/CS456 data output and sample number. To query the sensor for the configuration, use the **aV!** command followed by the **aD!** command.

The extended commands are used to select the temperature units (Celsius or Fahrenheit), pressure/level units (psig, kPa, bar, feet, meter, inches, or millimeter), and the integration time for each measurement. If level units are selected, they will represent level of fresh water. The multiplier (slope) and offset should be used to correct for relative density of water.

Sample number represents the number of values used to provide the output value received by the datalogger. This output value is an average of the samples.

The extended SDI-12 command used to configure output units is **aXCONFIG1=tt,pp,mmm.mm,ooo.oo!** where *a* = the SDI-12 address of the sensor, *tt* = temperature units, *pp* = measurement unit, *mmm.mm* = multiplier (slope), and *ooo.oo* = offset.

Valid entries for *tt* (temperature) are:

- 0 = Celsius
- 1 = Fahrenheit

and valid entries for pp (pressure/level) are:

- 0 = psig
- 1 = kPa
- 2 = bar
- 3 = feet
- 4 = meter
- 5 = inch
- 6 = millimeter

Only SDI-12 instruction **aM!**, **aM7!**, and **aM8!** output the results obtained when using the multiplier and offset. The multiplier and offset are only applied to the pressure/level value, not to the temperature.

The extended SDI-12 command used to configure sample number is **aXCONFIG2=nnn!**, where nnn is the number of samples that will be measured to obtain the final output value, which is an average of the samples taken. This value only applies to the **aM8!** command. The integration time is a result of the number of samples selected. This value can be derived by adding 2 s to the number of samples. For example, if nnn = 50, then 50 samples would be averaged. The integration time for this process is 50 plus 2, or 52 s.

# Appendix E. RS-232 Connection Via PC Terminal Software

---

PC terminal software can be used to communicate with the CS451/CS456 via the RS-232 communication mode (see FIGURE E-1).

The CS451/CS456 is connected to the PC via the A200 (see Section 8.1.1, *PC Connection Using the A200*).

Upon setup, the terminal emulator software will request you enter the Communication connection; defaults to a phone connection. Change the communication to appropriate “Com” in the “Connect Using” box (see Section 8.1.1.4, *Determining which COM Port the A200 has been Assigned*, to determine the COM port that was assigned to the A200). The software will then prompt for the proper “Port Settings”. TABLE E-1 shows the RS-232 settings.

TABLE E-1. RS-232 Settings	
Bits per Second	9600
Data bits	8
Parity	None
Stop bits	1
Flow control	None

You will now be able to communicate with the CS451/CS456. At the prompt, push the <Enter> key several times. This will wake-up the RS-232 mode of the sensor. TABLE E-2 shows the RS-232 commands that can be entered once it is in the RS-232 mode.

---

**NOTE**

By default, the CS451/CS456 is in the SDI-12 mode for communication. Once in the RS-232 mode, if there is no communication for 20 s, the sensor will return to the SDI-12 mode.

---

```
COM14 - PuTTY
CS451>
CS451>1
SerNum = 20010005
Water Level= 0.005375 feet
Therm= 25.134014 Degree C
SIG=0x96f0 Z
h
Copyright(C) Campbell Scientific Inc.
VERSION: CS451.Std.00  DATE: Feb 14,2012 4:50pm
 1 & 2 = Force Measurement and return the values
 3 = Force Meas & return DeltaR,Rb & Therm
 5 = Return SN, UserName & SDI12 address
 h = Help information
SIG=0xdb4 Z
5
Copyright(C) Campbell Scientific Inc.
VERSION: CS451.Std.00  DATE: Feb 14,2012 4:50pm
  SerNum = 20010005
  Element SN = 3110405
  Product Name = CS451- 2.9psig
  UserName = Pressure Sensor
  SDI12 Address = 0
SIG=0x2a98 Z
```

FIGURE E-1. Terminal Emulator

TABLE E-2. RS-232 Terminal Commands	
Terminal Commands	Values Returned
1	Serial Number, Pressure/Level, Temperature (in configured units)
2	Serial Number, Pressure (kPa), Temperature (°C)
3	Serial Number, ΔR(ohms), Rb(ohms), Temperature (°C), Element Serial Number, Product Name
5	Copyright information, OS Version and Date, Serial Number, Element Serial Number, Product Name, User Defined Name (Station Name), SDI-12 Address
H or h	Help menu



## Campbell Scientific Companies

---

**Campbell Scientific, Inc. (CSI)**

815 West 1800 North  
Logan, Utah 84321  
UNITED STATES

[www.campbellsci.com](http://www.campbellsci.com) • [info@campbellsci.com](mailto:info@campbellsci.com)

**Campbell Scientific Centro Caribe S.A. (CSCC)**

300 N Cementerio, Edificio Breller  
Santo Domingo, Heredia 40305  
COSTA RICA

[www.campbellsci.cc](http://www.campbellsci.cc) • [info@campbellsci.cc](mailto:info@campbellsci.cc)

**Campbell Scientific Africa Pty. Ltd. (CSAf)**

PO Box 2450  
Somerset West 7129  
SOUTH AFRICA

[www.csafrica.co.za](http://www.csafrica.co.za) • [cleroux@csafrica.co.za](mailto:cleroux@csafrica.co.za)

**Campbell Scientific Ltd. (CSL)**

Campbell Park  
80 Hathern Road  
Shepshed, Loughborough LE12 9GX  
UNITED KINGDOM

[www.campbellsci.co.uk](http://www.campbellsci.co.uk) • [sales@campbellsci.co.uk](mailto:sales@campbellsci.co.uk)

**Campbell Scientific Australia Pty. Ltd. (CSA)**

PO Box 8108  
Garbutt Post Shop QLD 4814  
AUSTRALIA

[www.campbellsci.com.au](http://www.campbellsci.com.au) • [info@campbellsci.com.au](mailto:info@campbellsci.com.au)

**Campbell Scientific Ltd. (CSL France)**

3 Avenue de la Division Leclerc  
92160 ANTONY  
FRANCE

[www.campbellsci.fr](http://www.campbellsci.fr) • [info@campbellsci.fr](mailto:info@campbellsci.fr)

**Campbell Scientific (Beijing) Co., Ltd.**

8B16, Floor 8 Tower B, Hanwei Plaza  
7 Guanghua Road  
Chaoyang, Beijing 100004  
P.R. CHINA

[www.campbellsci.com](http://www.campbellsci.com) • [info@campbellsci.com.cn](mailto:info@campbellsci.com.cn)

**Campbell Scientific Ltd. (CSL Germany)**

Fahrenheitstraße 13  
28359 Bremen  
GERMANY

[www.campbellsci.de](http://www.campbellsci.de) • [info@campbellsci.de](mailto:info@campbellsci.de)

**Campbell Scientific do Brasil Ltda. (CSB)**

Rua Apinagés, n.br. 2018 — Perdizes  
CEP: 01258-00 — São Paulo — SP  
BRASIL

[www.campbellsci.com.br](http://www.campbellsci.com.br) • [vendas@campbellsci.com.br](mailto:vendas@campbellsci.com.br)

**Campbell Scientific Spain, S. L. (CSL Spain)**

Avda. Pompeu Fabra 7-9, local 1  
08024 Barcelona  
SPAIN

[www.campbellsci.es](http://www.campbellsci.es) • [info@campbellsci.es](mailto:info@campbellsci.es)

**Campbell Scientific Canada Corp. (CSC)**

14532 – 131 Avenue NW  
Edmonton AB T5L 4X4  
CANADA

[www.campbellsci.ca](http://www.campbellsci.ca) • [dataloggers@campbellsci.ca](mailto:dataloggers@campbellsci.ca)

Please visit [www.campbellsci.com](http://www.campbellsci.com) to obtain contact information for your local US or international representative.